

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012325\
Data File : BF141245.D
Acq On : 23 Jan 2025 13:07
Operator : RC/JU
Sample : PB166185BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166185BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	560	567	572	rBV	3493515	4901683	63.19%	12.008%
2	6.434	731	738	743	rBV	3395954	4956186	63.89%	12.141%
3	6.804	796	801	806	rBV	872580	1062253	13.69%	2.602%
4	7.363	889	896	902	rBV	2289985	3309690	42.67%	8.108%
5	8.087	1013	1019	1024	rBV	1104566	1453836	18.74%	3.562%
6	9.163	1195	1202	1208	rBV	4506066	6442060	83.05%	15.781%
7	9.845	1311	1318	1323	rBV	1321556	1736835	22.39%	4.255%
8	10.634	1445	1452	1475	rBV	3220415	4516565	58.22%	11.064%
9	11.333	1565	1571	1576	rBV	1486095	1855902	23.93%	4.547%
10	12.927	1835	1842	1847	rBV	5628417	7757158	100.00%	19.003%
11	13.980	2016	2021	2031	rBV	1189921	1619014	20.87%	3.966%
12	15.469	2268	2274	2281	rBV	759117	1209261	15.59%	2.962%




Sum of corrected areas: 40820443

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012325\
Data File : BF141245.D
Acq On : 23 Jan 2025 13:07
Operator : RC/JU
Sample : PB166185BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166185BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

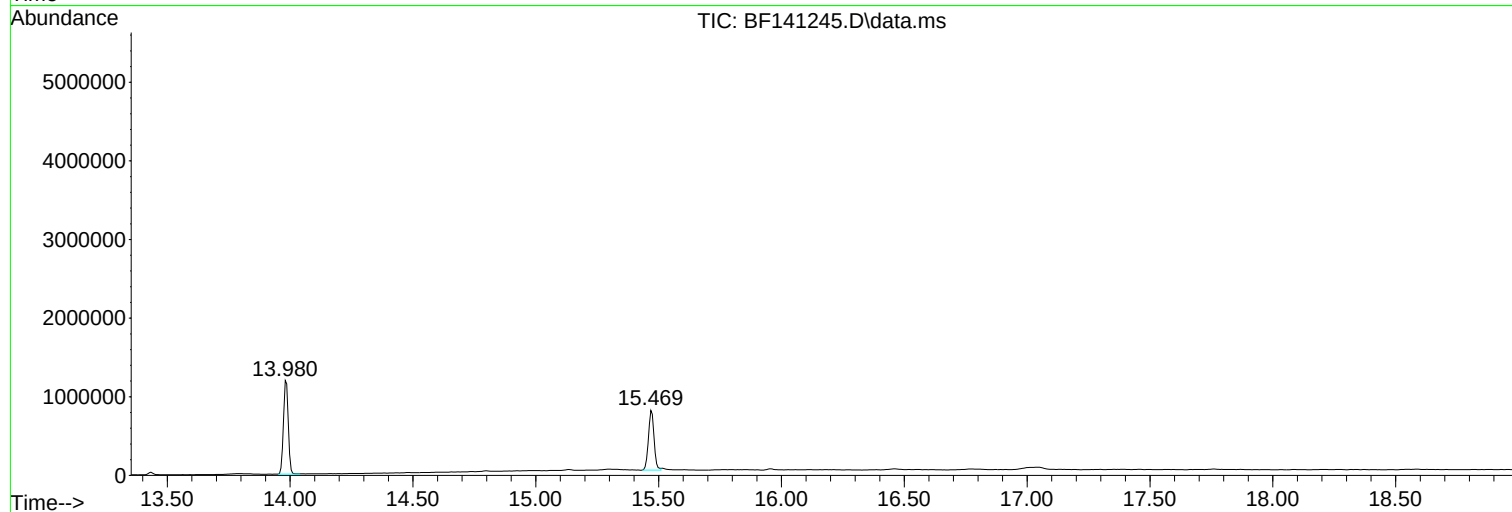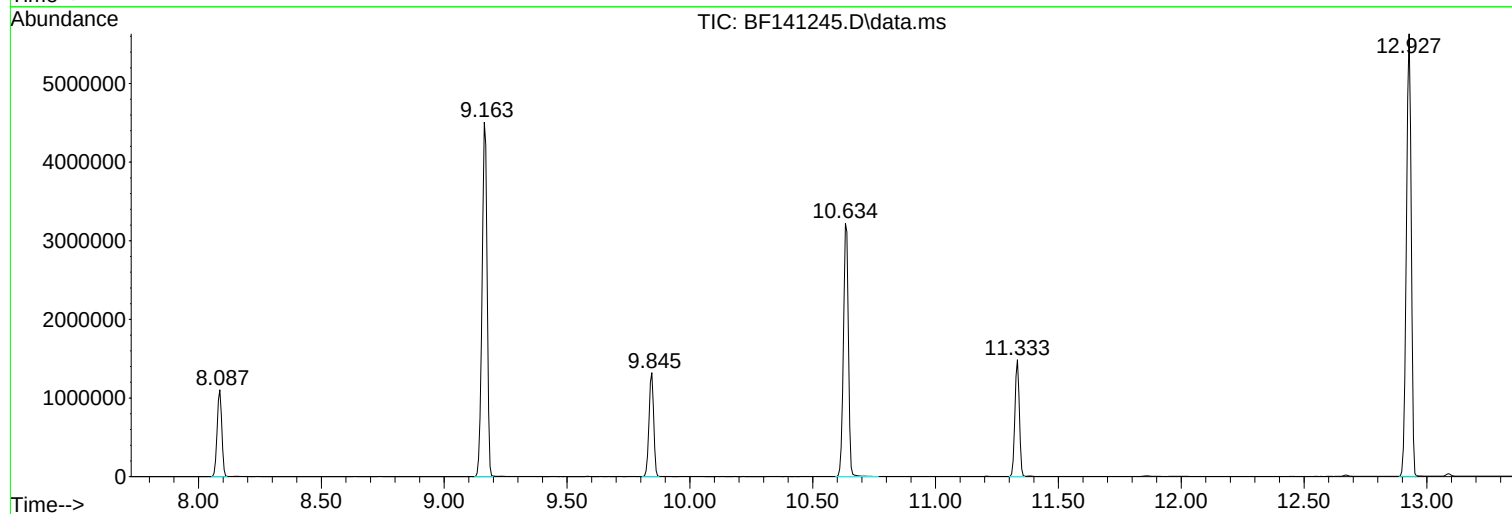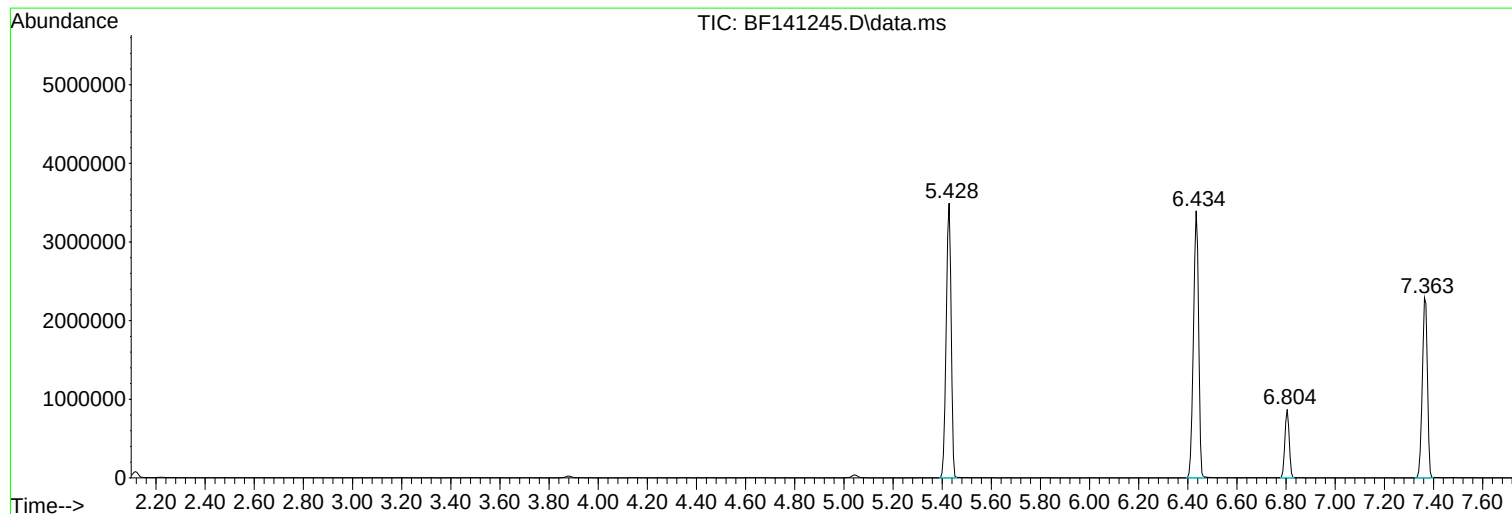

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012325\
Data File : BF141245.D
Acq On : 23 Jan 2025 13:07
Operator : RC/JU
Sample : PB166185BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166185BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012325\
Data File : BF141245.D
Acq On : 23 Jan 2025 13:07
Operator : RC/JU
Sample : PB166185BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166185BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------