

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012325\
 Data File : BF141247.D
 Acq On : 23 Jan 2025 13:59
 Operator : RC/JU
 Sample : PB166188BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166188BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	3	5	11	rVB	73021	87475	1.17%	0.221%
2	5.428	560	567	572	rBV	3505770	4970316	66.39%	12.560%
3	6.434	731	738	743	rBV	3412633	5022412	67.08%	12.692%
4	6.804	796	801	806	rBV	762819	944518	12.62%	2.387%
5	7.363	889	896	902	rBV	2327109	3385665	45.22%	8.556%
6	8.086	1012	1019	1024	rBV	957332	1282832	17.13%	3.242%
7	9.163	1195	1202	1208	rBV	4522655	6498185	86.79%	16.421%
8	9.839	1311	1317	1323	rBV	1138576	1524692	20.36%	3.853%
9	10.633	1445	1452	1457	rBV	3347401	4491645	59.99%	11.350%
10	11.327	1565	1570	1576	rBV	1222494	1618225	21.61%	4.089%
11	12.927	1835	1842	1847	rBV	5283830	7486904	100.00%	18.920%
12	13.980	2016	2021	2030	rBV	988915	1312013	17.52%	3.315%
13	15.468	2268	2274	2280	rBV	580972	947516	12.66%	2.394%




Sum of corrected areas: 39572398

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012325\
Data File : BF141247.D
Acq On : 23 Jan 2025 13:59
Operator : RC/JU
Sample : PB166188BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166188BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

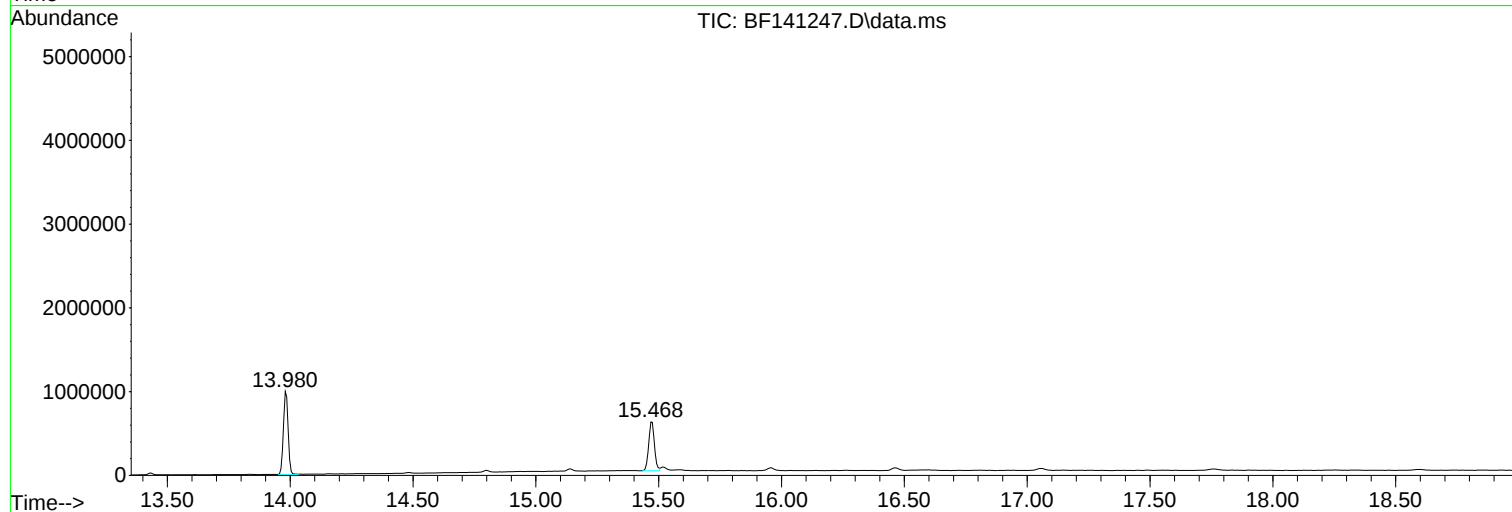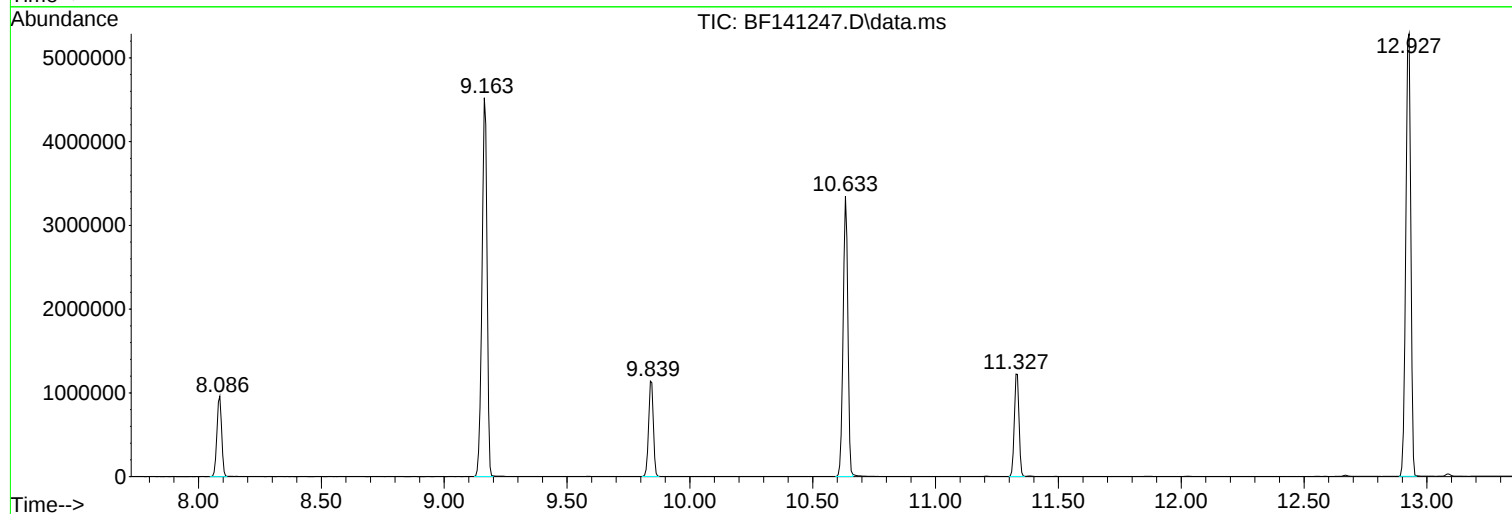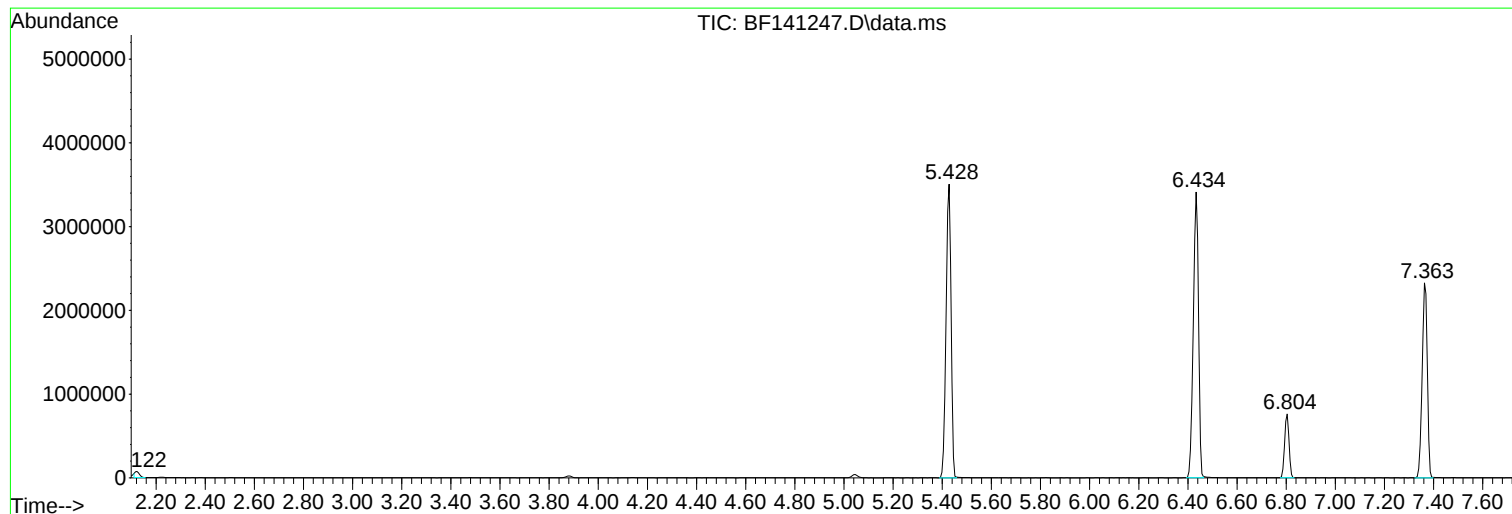

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012325\
Data File : BF141247.D
Acq On : 23 Jan 2025 13:59
Operator : RC/JU
Sample : PB166188BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166188BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012325\
Data File : BF141247.D
Acq On : 23 Jan 2025 13:59
Operator : RC/JU
Sample : PB166188BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166188BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------