


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012325\
Data File : BF141243.D
Acq On : 23 Jan 2025 12:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

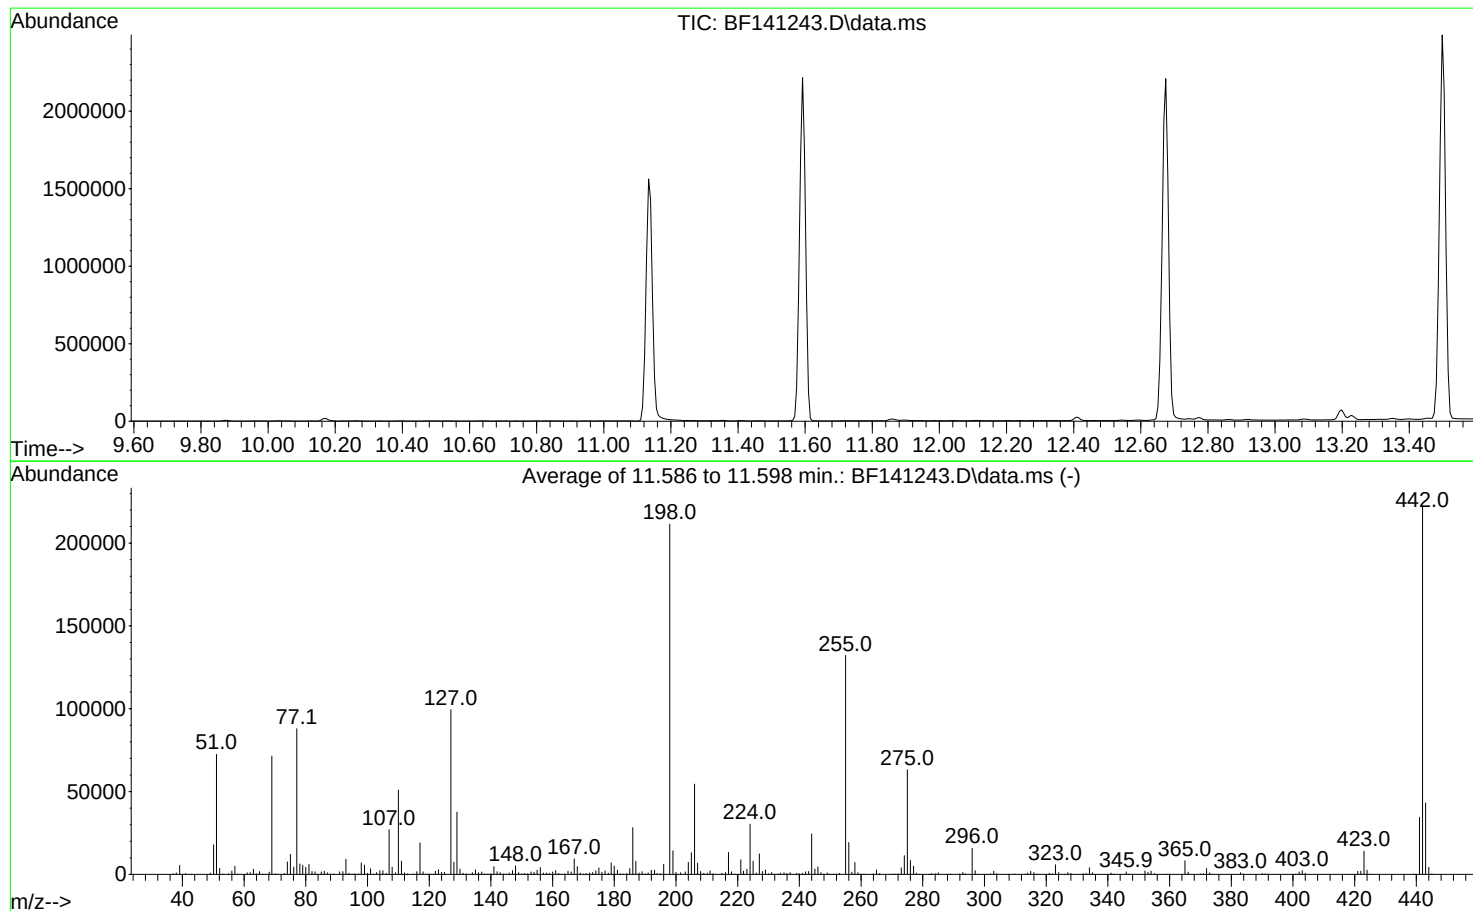

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	72509	PASS
68	69	0.00	2	1.9	1392	PASS
69	198	0.00	100	33.8	71429	PASS
70	69	0.00	2	0.6	421	PASS
127	198	10	80	47.0	99451	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	211456	PASS
199	198	5	9	6.7	14166	PASS
275	198	10	60	29.9	63219	PASS
365	198	1	100	3.9	8183	PASS
441	198	0.01	100	16.3	34413	PASS
442	442	50	100	100.0	222123	PASS
443	442	15	24	19.4	43123	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/23/2025	BNA_F	<u>BF141243.D</u>
Compound Name	Response	Retention Time
DDT	646634	13.498
DDD	24235	13.198
DDE	1150	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25385	672019	3.78

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012325\
Data File : BF141243.D
Acq On : 23 Jan 2025 12:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 23 13:22:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

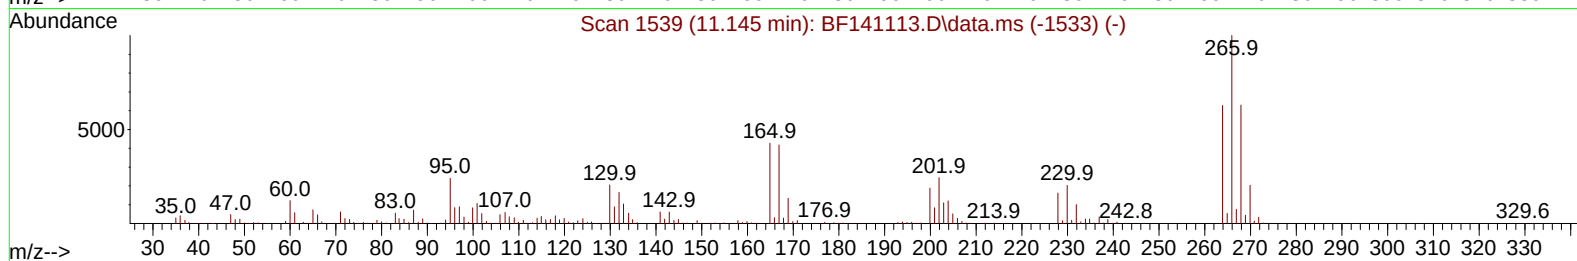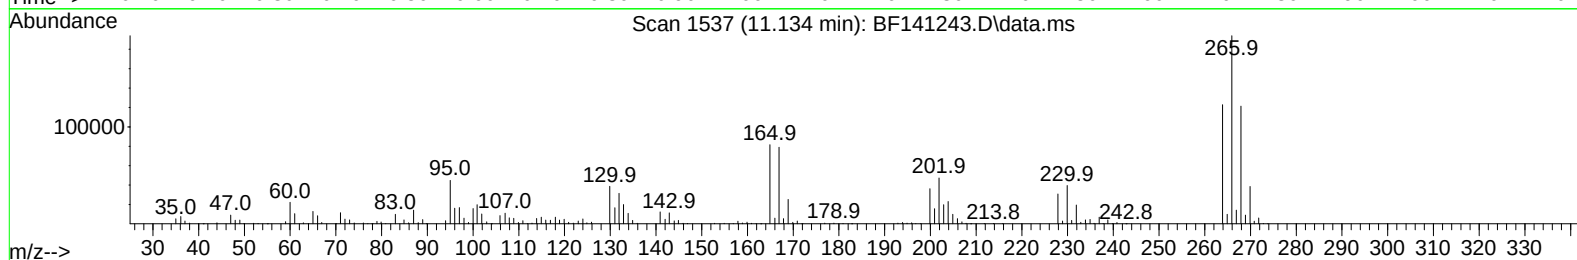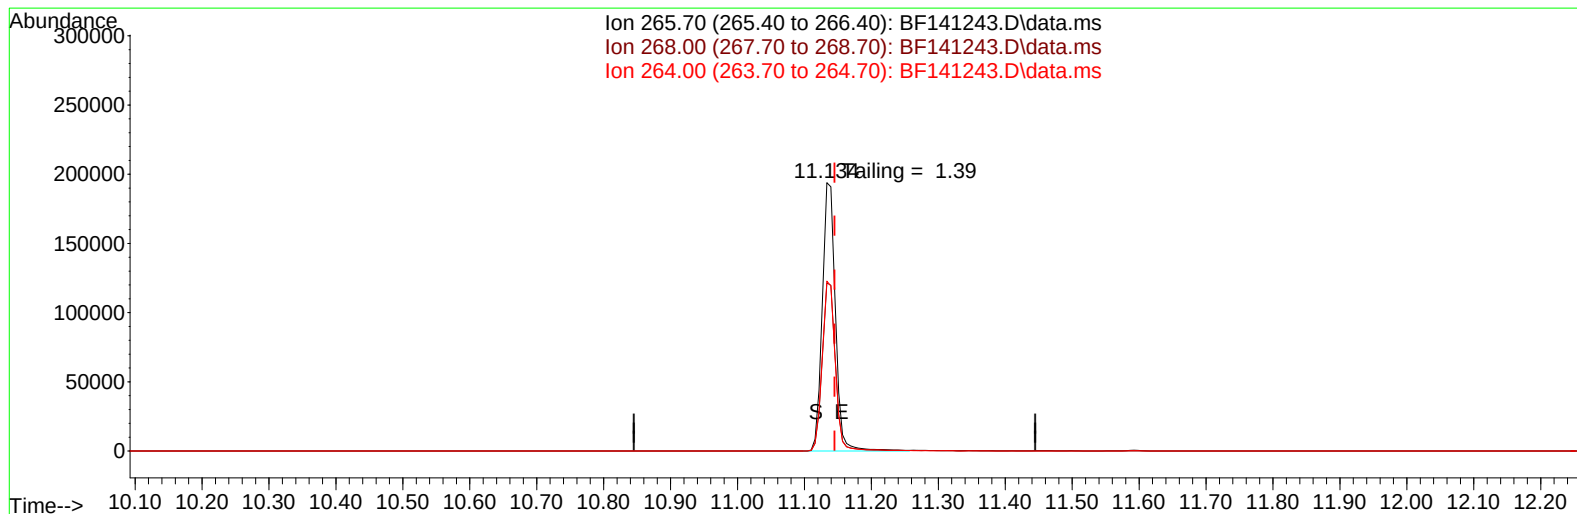

TIC: BF141243.D\data.ms

(70) Pentachlorophenol (C)

11.134min (-0.012) 29408.38 ng




response 265988

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.61
264.00	62.70	63.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012325\
Data File : BF141243.D
Acq On : 23 Jan 2025 12:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 23 13:22:52 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

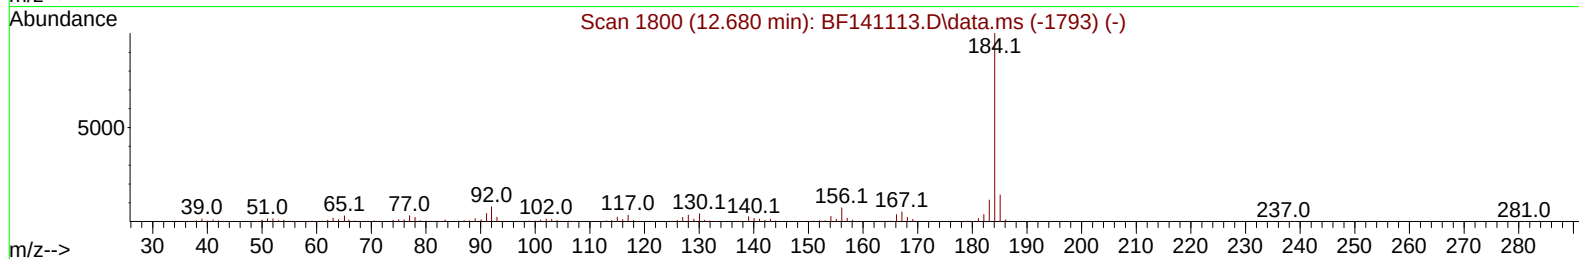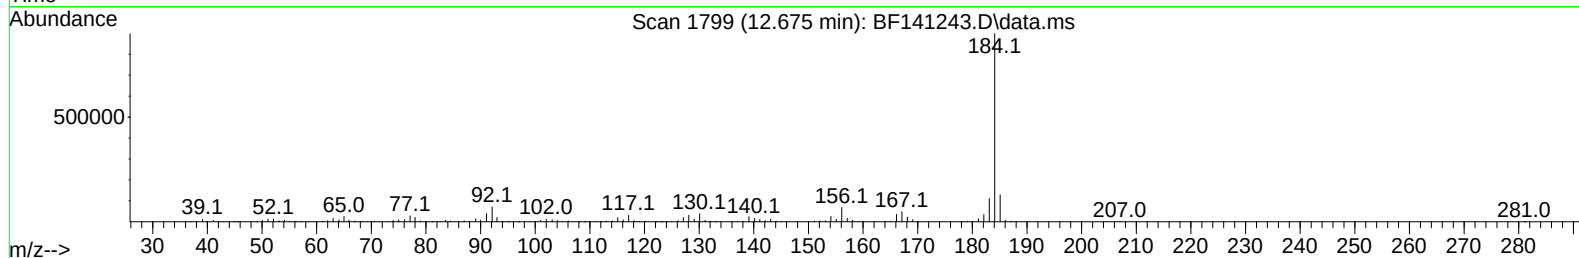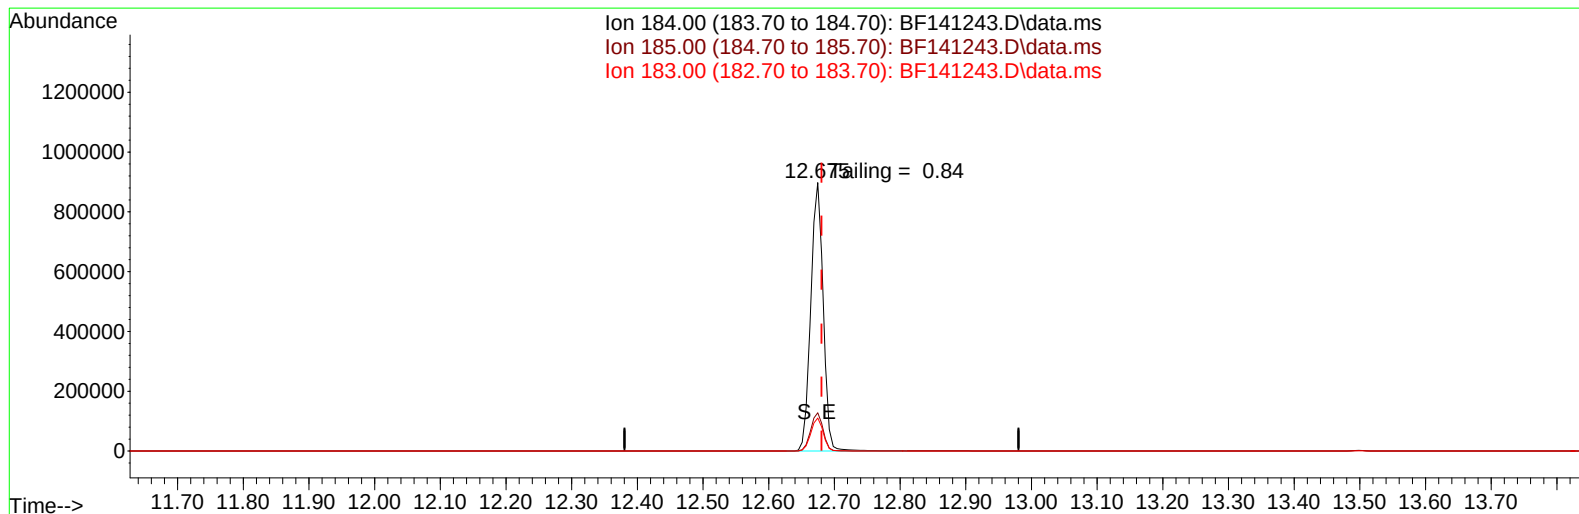

TIC: BF141243.D\data.ms

(77) Benzidine

12.675min (-0.006) 67921.69 ng

response 1180213

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.29
183.00	11.50	12.33
0.00	0.00	0.00