
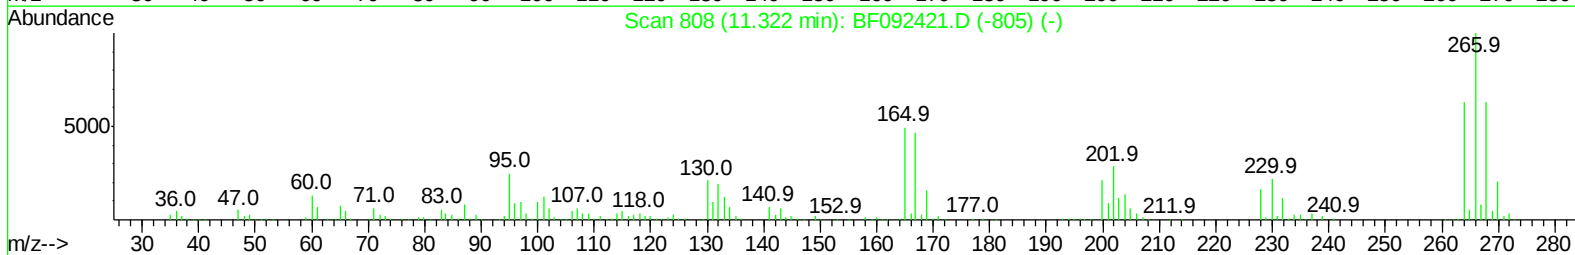
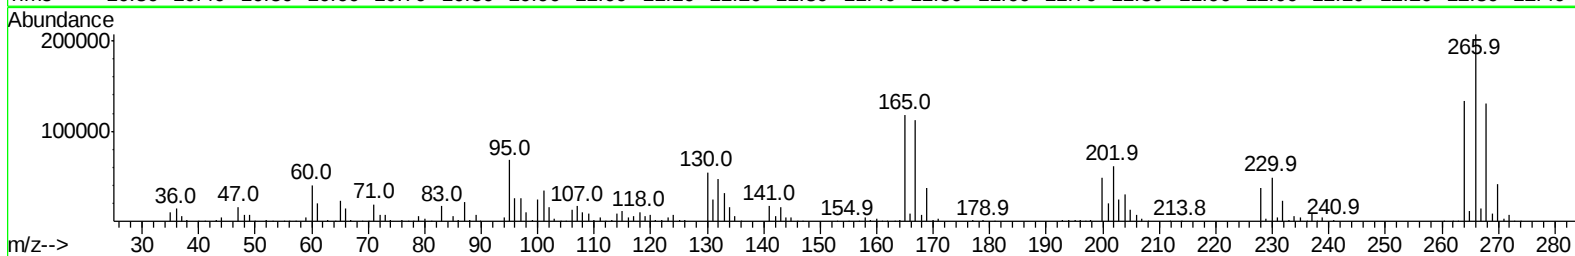


Data Path : Z:\HPCHEM1\BNA F\DATA\BF012417\
Data File : BF092417.D
Acq On : 24 Jan 2017 9:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 15:10:35 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

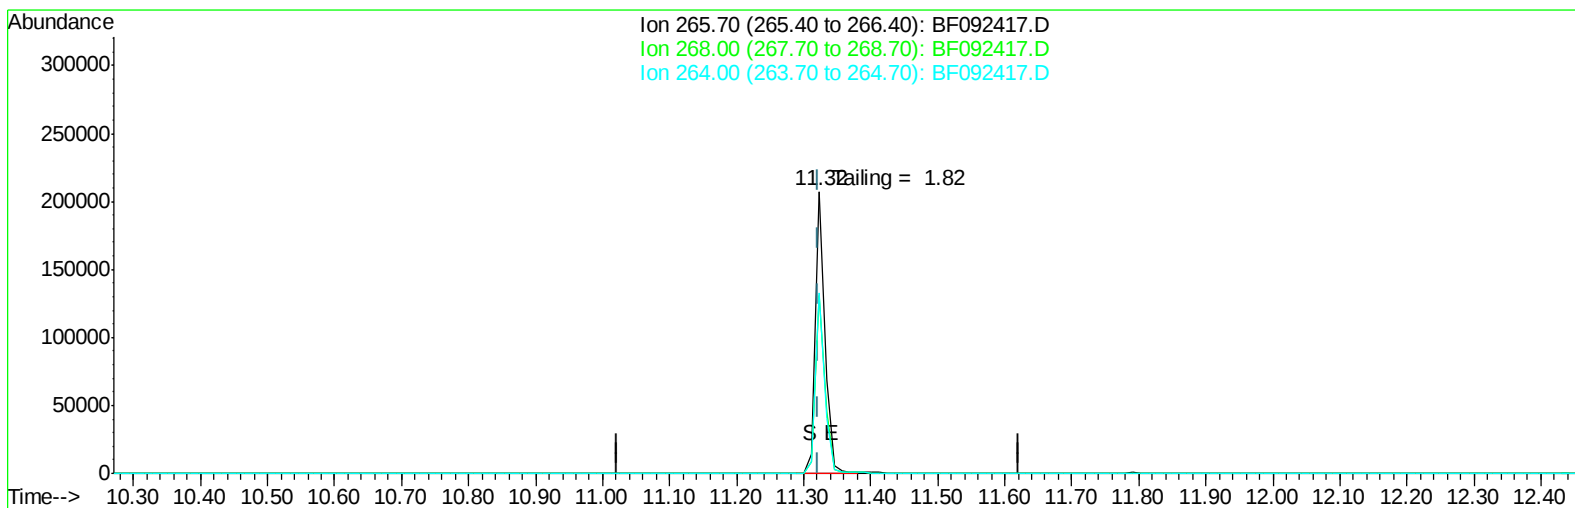

TIC: BF092417.D

(69) Pentachlorophenol (C)




11.322min (+0.000) 0.00ng

response 208038

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	63.17
264.00	62.90	64.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012417\
Data File : BF092417.D
Acq On : 24 Jan 2017 9:44
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 15:10:35 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

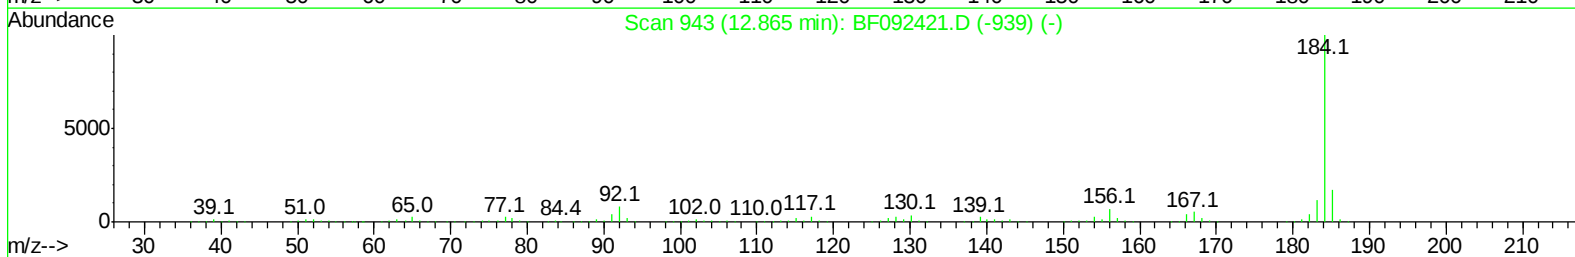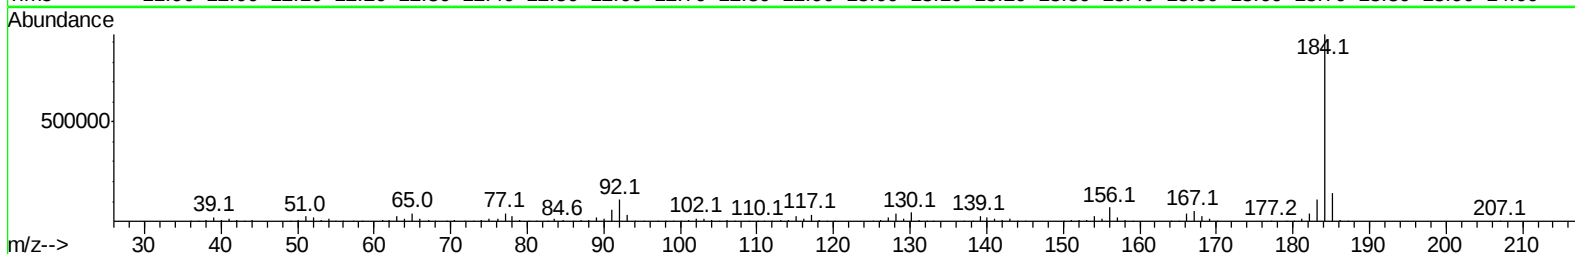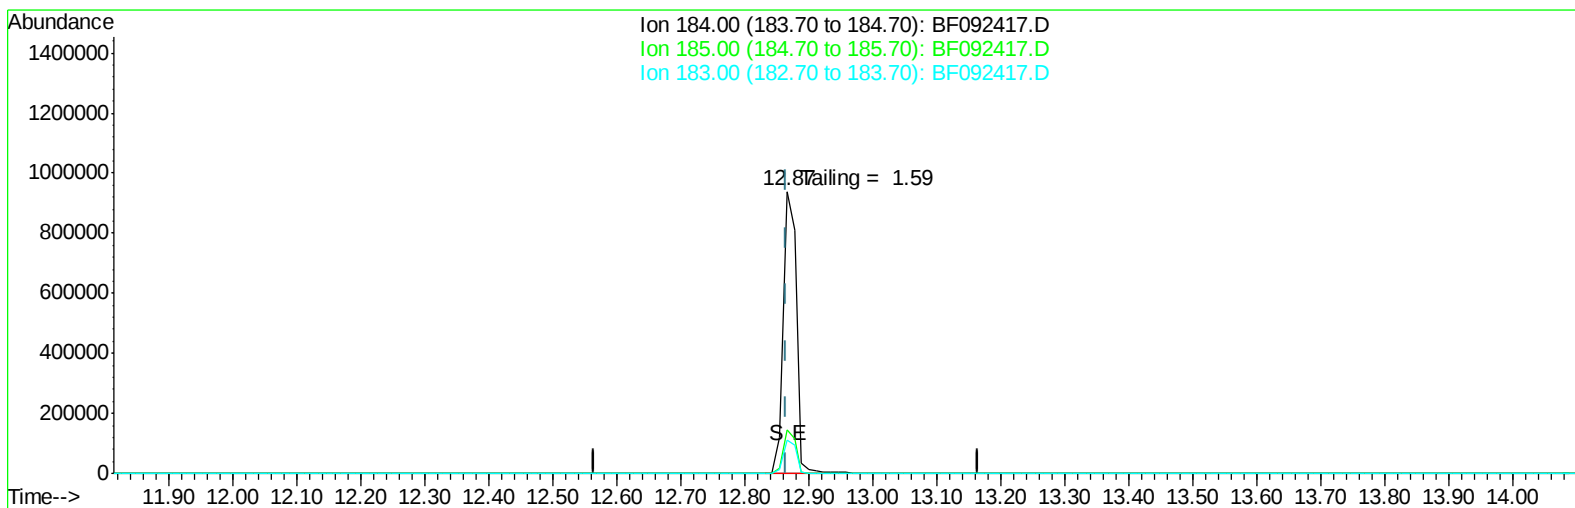

TIC: BF092417.D

(76) Benzidine

12.865min (+0.000) 48945.34ng

response 1335501

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.25
183.00	11.50	12.01
0.00	0.00	0.00