
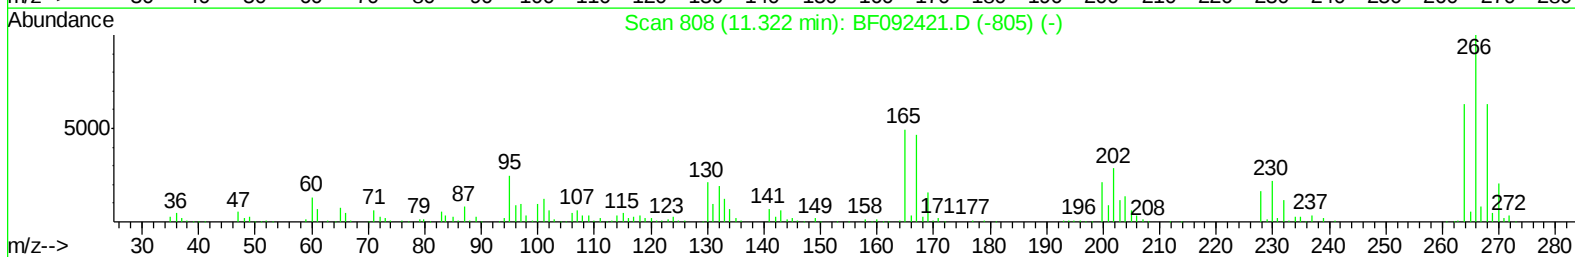
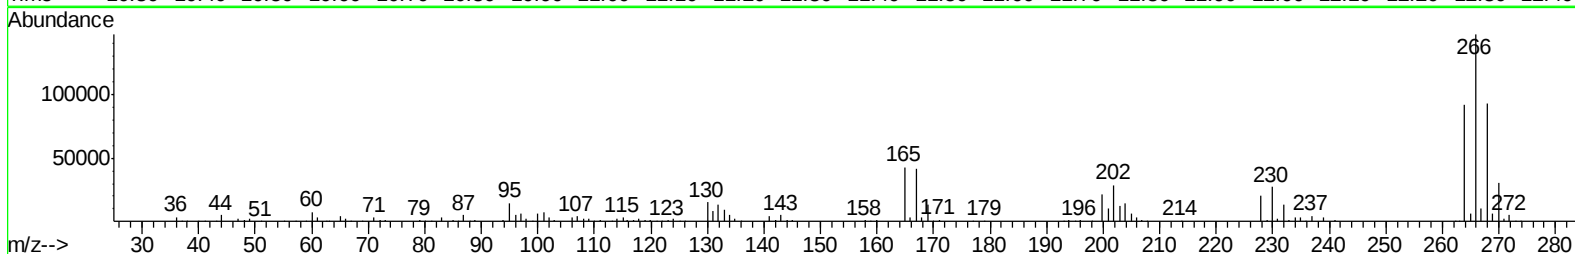


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012417\
Data File : BF092437.D
Acq On : 24 Jan 2017 19:05
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 06:43:37 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

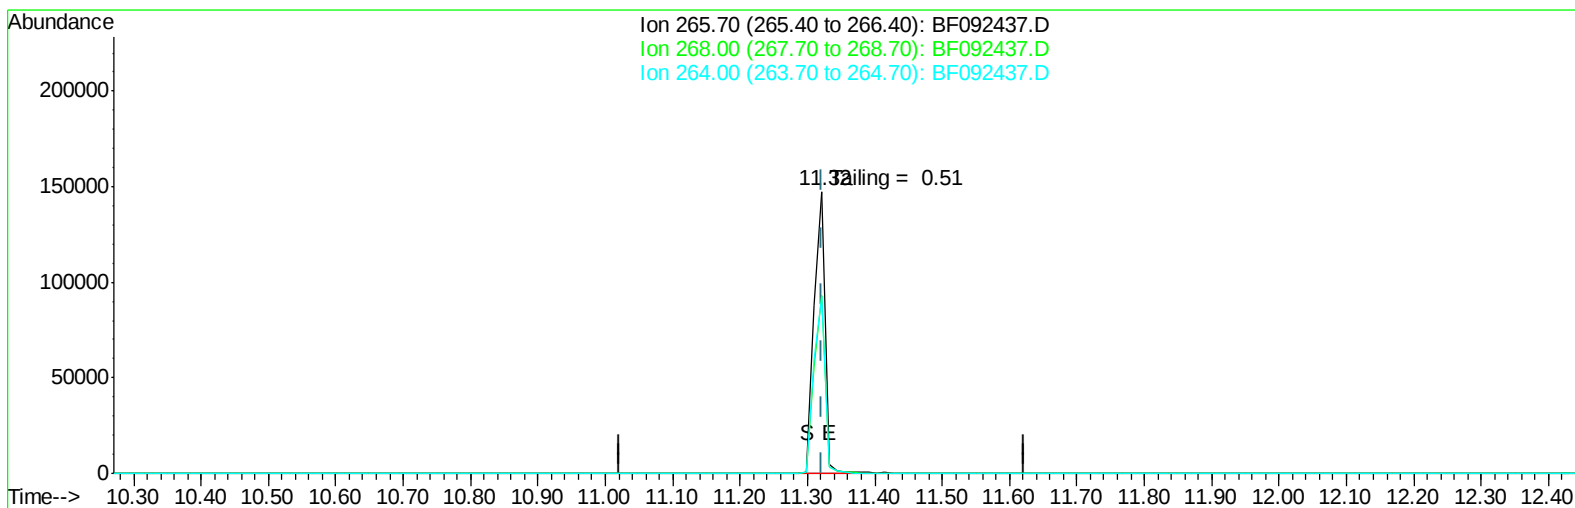

TIC: BF092437.D

(69) Pentachlorophenol (C)




11.322min (-0.000) 0.00ng

response 168488

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	63.13
264.00	62.90	62.62
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012417\
Data File : BF092437.D
Acq On : 24 Jan 2017 19:05
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 06:43:37 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

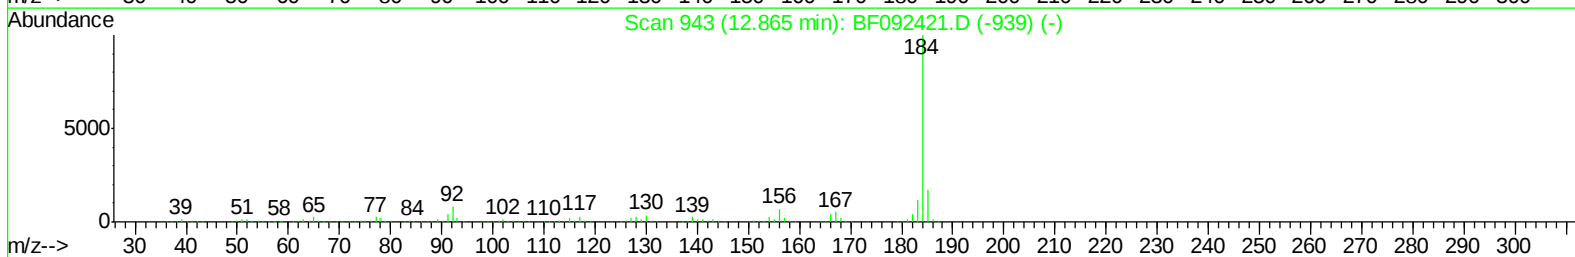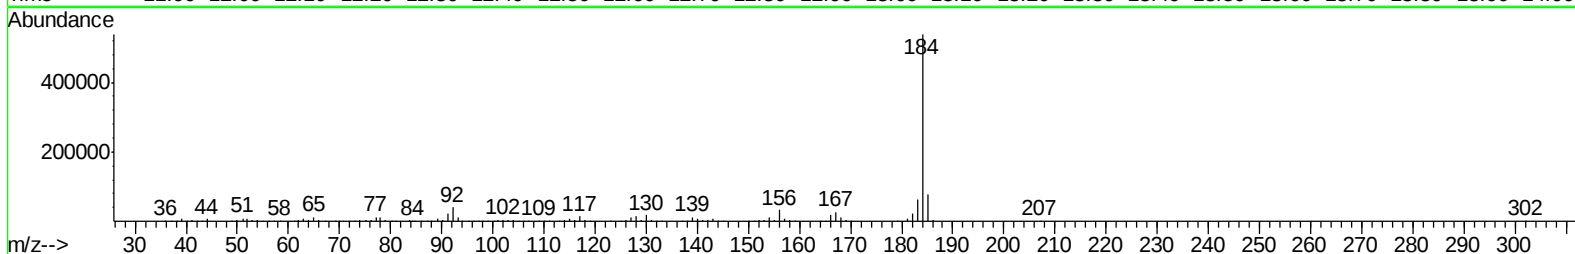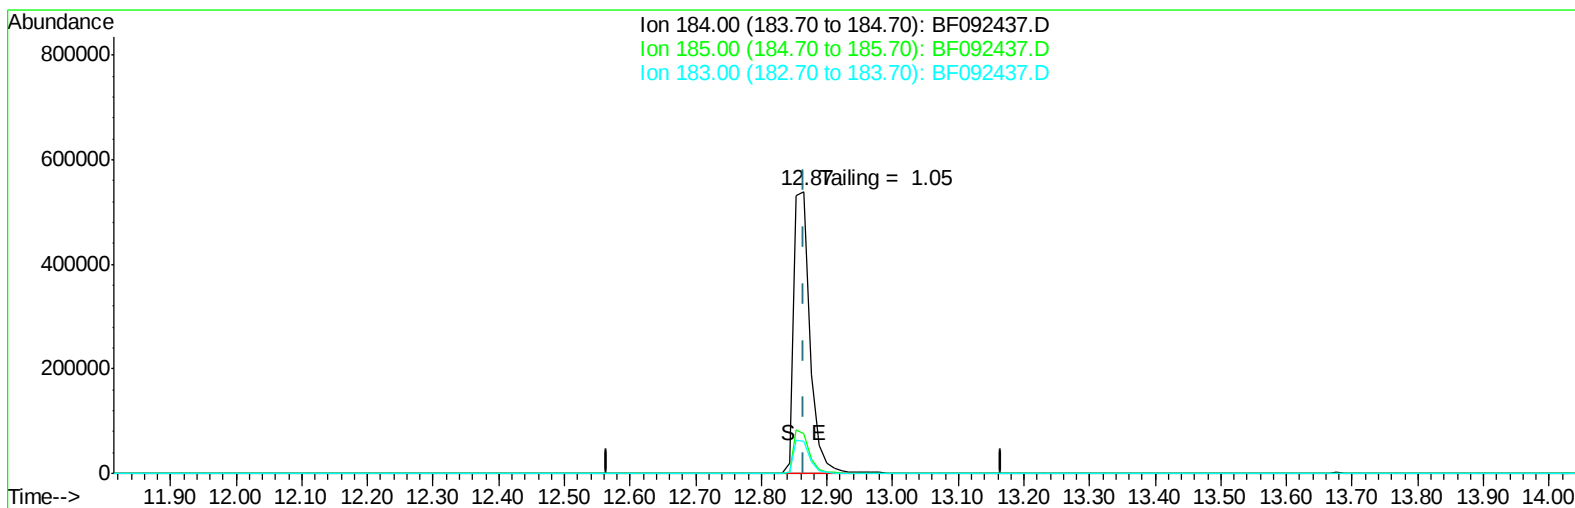

TIC: BF092437.D

(76) Benzidine

12.865min (-0.000) 0.00ng

response 949269

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.18
183.00	11.50	11.58
0.00	0.00	0.00