

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012417\
 Data File : BF092428.D
 Acq On : 24 Jan 2017 14:50
 Operator : UM/SJ
 Sample : I1305-25
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 0036

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.236	11	13	31	rVB4	85822	291796	3.05%	0.144%
2	3.424	109	117	120	rBV	924001	3274532	34.20%	1.611%
3	5.162	266	269	281	rVB	1556007	2331144	24.35%	1.147%
4	5.573	301	305	307	rBV	4319991	5427999	56.70%	2.670%
5	6.590	390	394	397	rBV	3617178	5237954	54.71%	2.576%
6	6.705	401	404	405	rBV	3022236	2888952	30.18%	1.421%
7	6.739	405	407	409	rVB	4387694	4865611	50.82%	2.393%
8	6.910	419	422	424	rBV	1623723	1398317	14.61%	0.688%
9	6.990	425	429	431	rBV2	3864023	4635580	48.42%	2.280%
10	7.150	438	443	445	rBV2	5061609	9245349	96.57%	4.547%
11	7.390	460	464	467	rBV	3730754	5858980	61.20%	2.882%
12	7.493	470	473	474	rBV	3446941	3760570	39.28%	1.850%
13	7.539	474	477	480	rVB2	2871692	4565504	47.69%	2.245%
14	7.802	496	500	502	rBV	4949800	6213339	64.90%	3.056%
15	8.008	515	518	521	rBV	1599260	1908058	19.93%	0.938%
16	8.202	532	535	538	rBV	3269751	3927502	41.02%	1.932%
17	8.293	538	543	545	rVV	5456117	8632755	90.17%	4.246%
18	8.785	583	586	588	rVB	197902	214136	2.24%	0.105%
19	8.979	600	603	606	rBV	3864995	5329213	55.66%	2.621%
20	9.139	614	617	619	rBV	2668114	2949838	30.81%	1.451%
21	9.345	632	635	638	rVB	3600634	5737634	59.93%	2.822%
22	9.471	643	646	649	rVB	3568889	5702200	59.56%	2.805%
23	9.893	679	683	685	rBV	5166933	5613464	58.63%	2.761%
24	10.031	692	695	696	rBV	1473699	1752163	18.30%	0.862%
25	10.076	696	699	701	rVB	5995027	9046618	94.49%	4.449%
26	10.202	708	710	713	rVB	886275	865016	9.04%	0.425%
27	10.453	728	732	734	rBV	3131923	2827501	29.53%	1.391%
28	10.579	740	743	745	rVB	3196001	3836246	40.07%	1.887%
29	10.694	750	753	755	rVB	2875591	3006728	31.41%	1.479%
30	10.819	761	764	767	rBV	2511806	2683653	28.03%	1.320%
31	11.071	783	786	788	rVB	2687425	3347395	34.96%	1.646%
32	11.414	810	816	818	rVB	89430	107332	1.12%	0.053%
33	11.551	823	828	830	rBV2	5410685	8963190	93.62%	4.408%
34	11.608	830	833	835	rVB	5828694	6619842	69.15%	3.256%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012417\
 Data File : BF092428.D
 Acq On : 24 Jan 2017 14:50
 Operator : UM/SJ
 Sample : I1305-25
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 0036

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.745	843	845	847	rVB	135353	114112	1.19%	0.056%
36	12.088	873	875	878	rVB	3702013	4908069	51.27%	2.414%
37	12.305	892	894	899	rBV2	309995	472664	4.94%	0.232%
38	13.117	962	965	967	rBV	4158034	5149059	53.78%	2.533%
39	13.597	1004	1007	1009	rBV	6076415	7144874	74.63%	3.514%
40	14.168	1053	1057	1058	rBV	5506011	9573749	100.00%	4.709%
41	14.202	1058	1060	1063	rVB	5013527	5931684	61.96%	2.917%
42	14.762	1106	1109	1112	rBV	4604063	5507648	57.53%	2.709%
43	15.243	1147	1151	1154	rBV	3225941	6011420	62.79%	2.957%
44	15.300	1154	1156	1162	rVB2	52644	103556	1.08%	0.051%
45	15.631	1182	1185	1188	rBV	521182	782203	8.17%	0.385%
46	17.163	1310	1319	1327	rBV2	2316281	7724067	80.68%	3.799%
47	17.620	1350	1359	1362	rBV	2002155	6828755	71.33%	3.359%


Sum of corrected areas: 203317971

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012417\
Data File : BF092428.D
Acq On : 24 Jan 2017 14:50
Operator : UM/SJ
Sample : I1305-25
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
0036

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

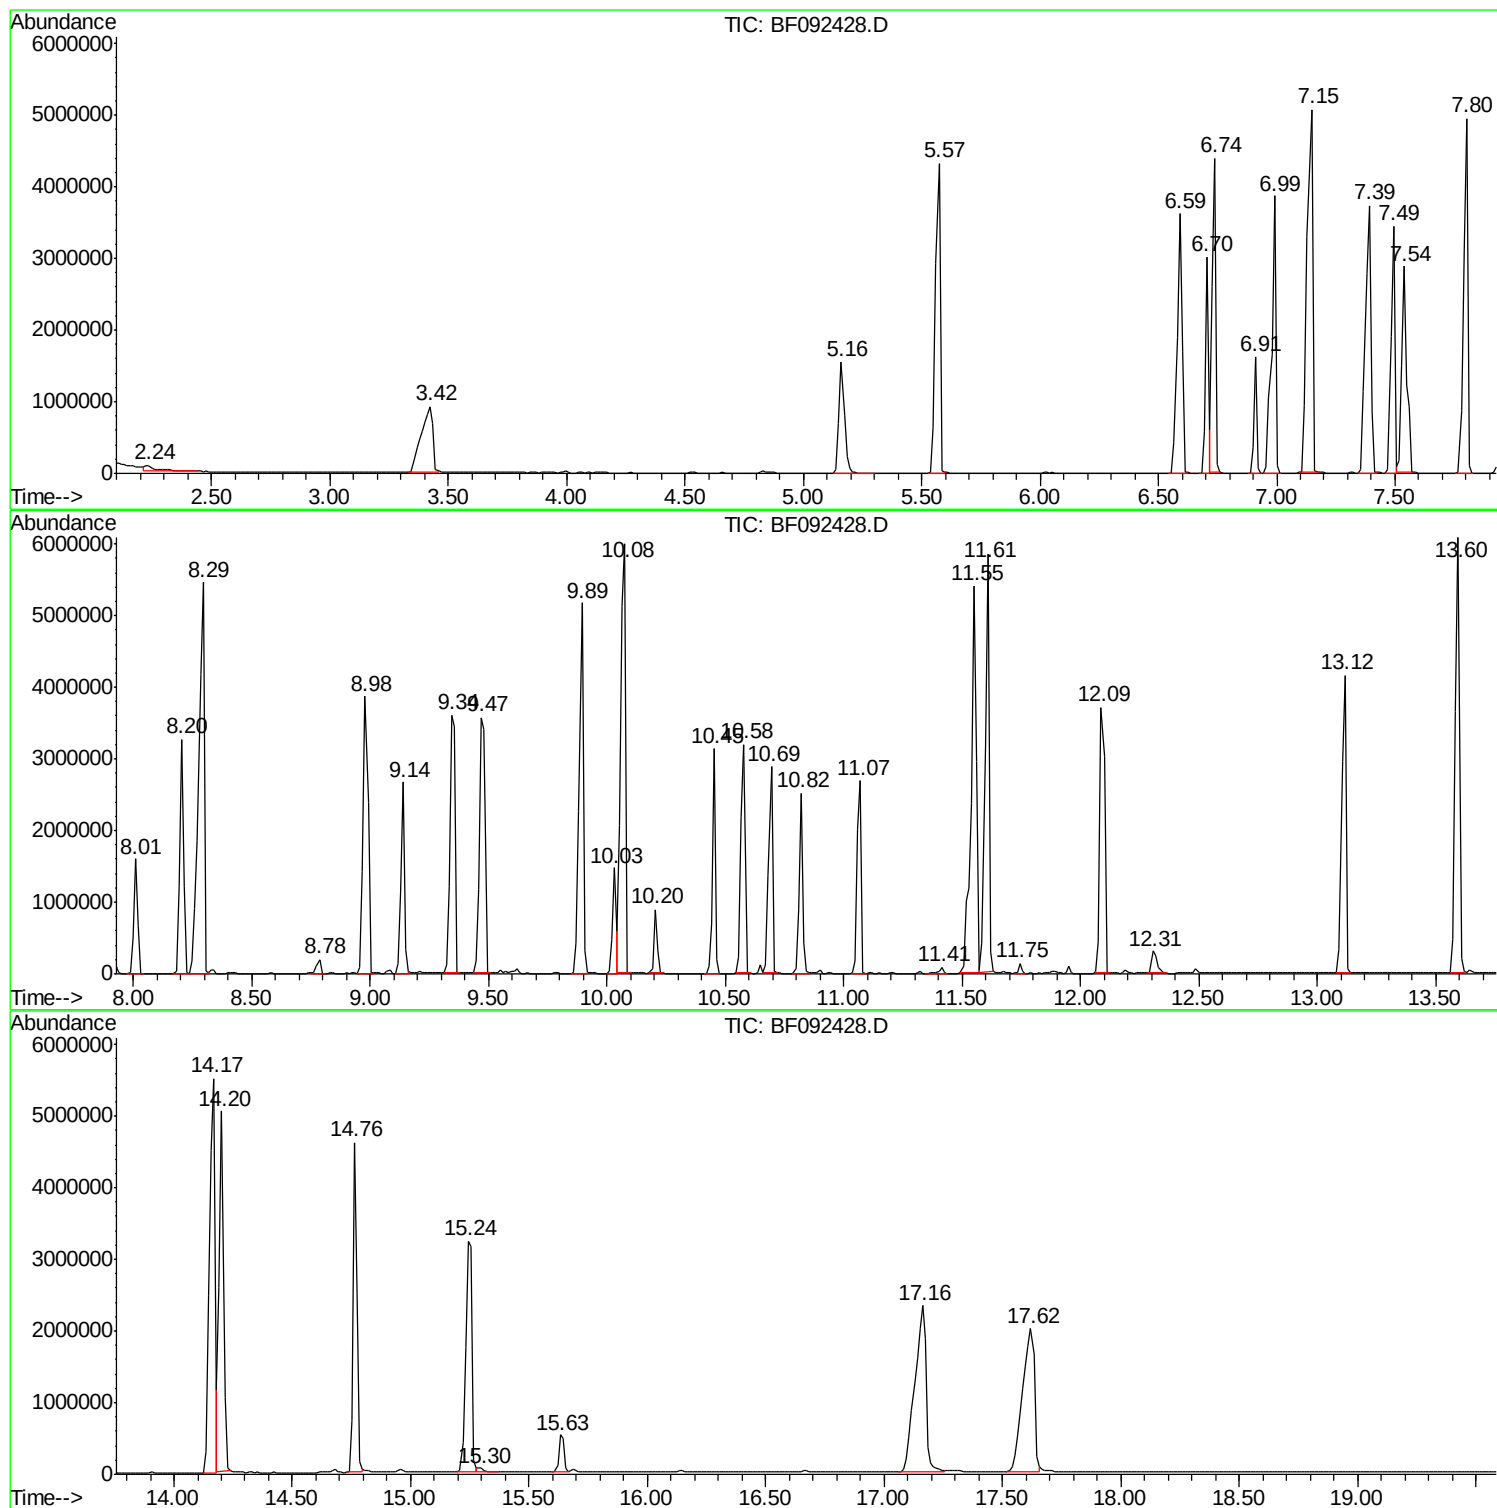

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012417\
Data File : BF092428.D
Acq On : 24 Jan 2017 14:50
Operator : UM/SJ
Sample : I1305-25
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
0036










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.16	10.06 ng	2331140	1,4-Dichlorobenzene-d4	6.97

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16
3		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4		Acetic acid, 2-propenyl ester	100	C5H8O2	000591-87-7	9
5		Formamide, N,N-diethyl-	101	C5H11NO	000617-84-5	7

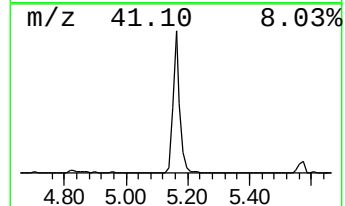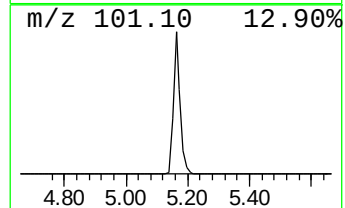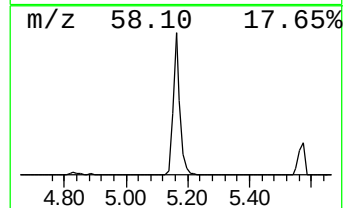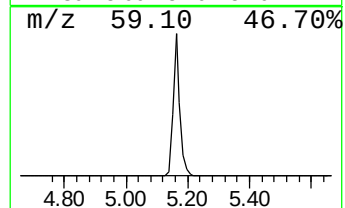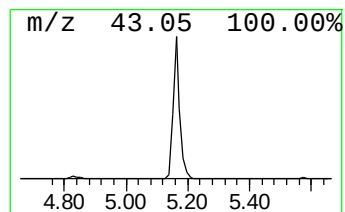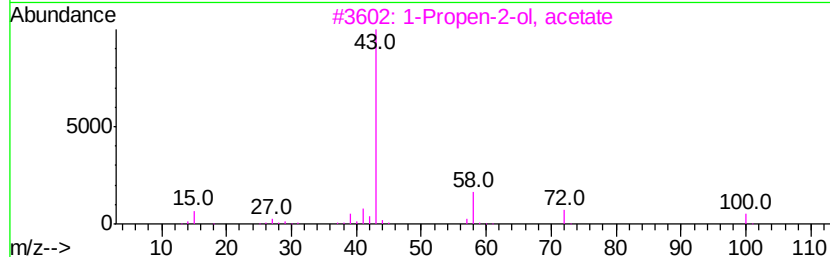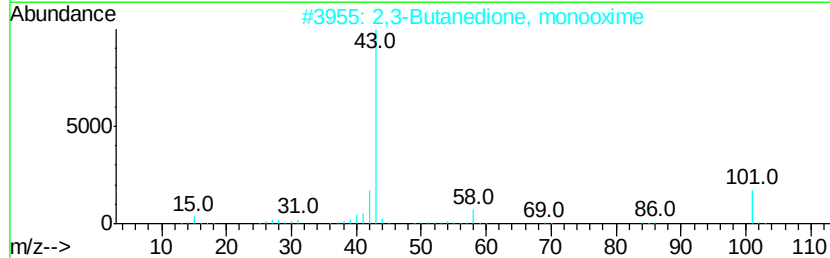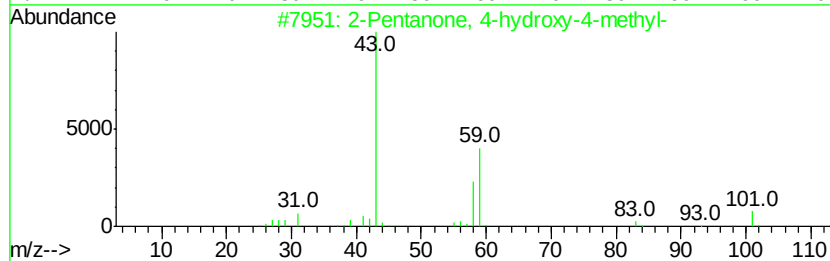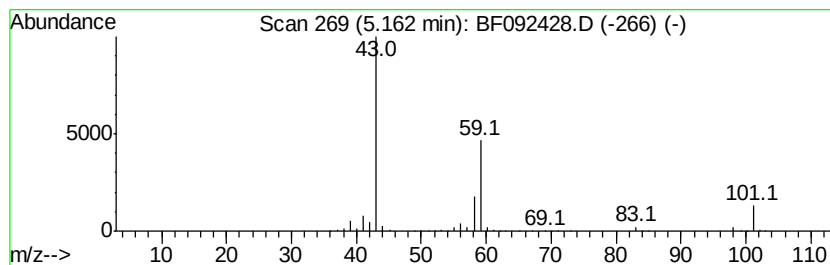

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012417\
Data File : BF092428.D
Acq On : 24 Jan 2017 14:50
Operator : UM/SJ
Sample : I1305-25
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
0036

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.16	10.1	ng	2331140	1	6.97	4635580	20.0