


Data Path : Z:\HPCHEM1\BNA F\DATA\BF012417\
 Data File : BF092417.D
 Acq On : 24 Jan 2017 9:44
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 24 13:48:07 2017

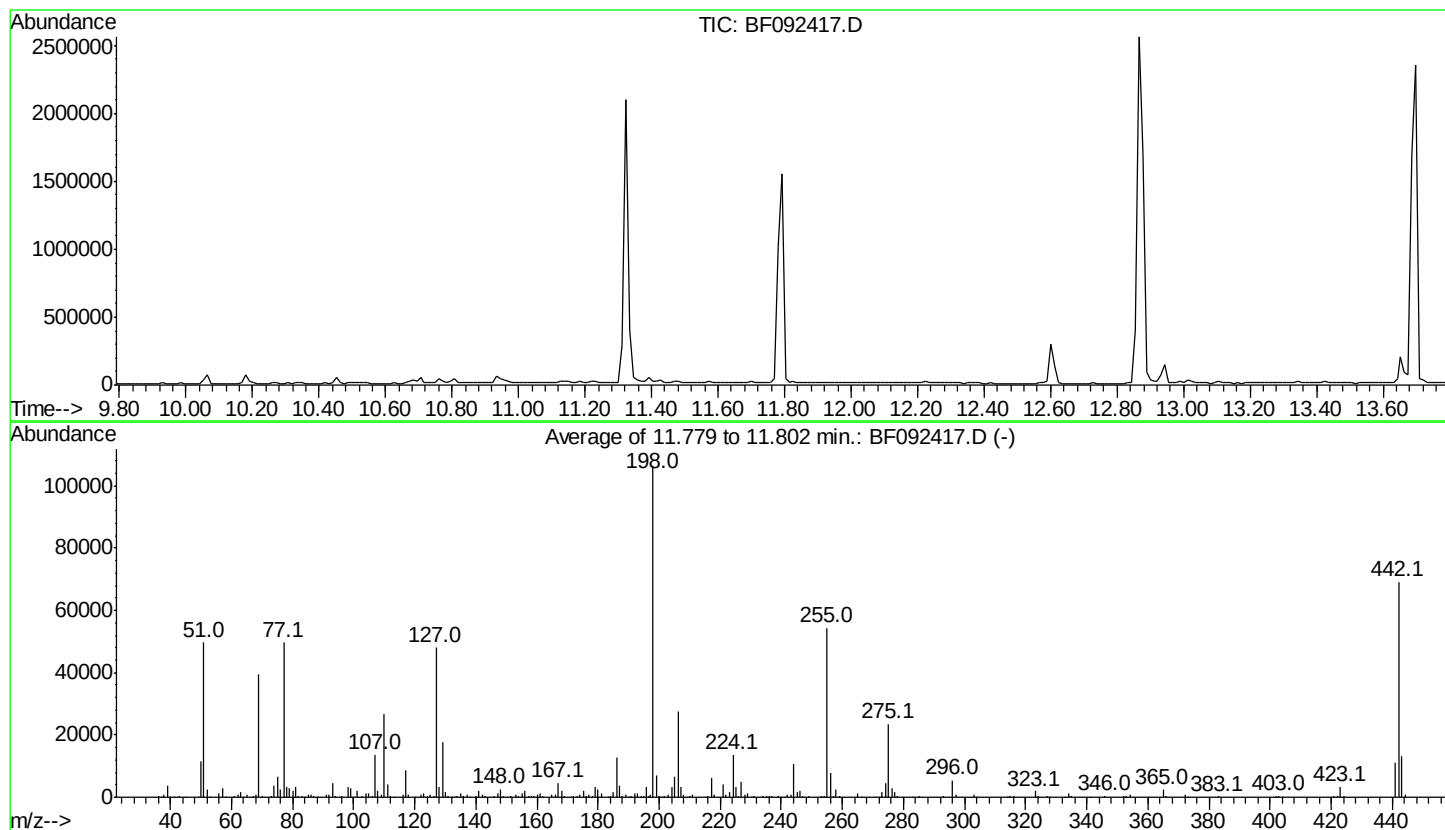

AutoFind: Scans 848, 849, 850; Background Corrected with Scan 844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.7	49731	PASS
68	69	0.00	2	1.9	730	PASS
69	198	0.00	100	36.9	39326	PASS
70	69	0.00	2	1.1	425	PASS
127	198	10	80	45.0	47935	PASS
197	198	0.00	2	0.7	728	PASS
198	198	100	100	100.0	106470	PASS
199	198	5	9	6.5	6967	PASS
275	198	10	60	22.1	23520	PASS
365	198	1	100	2.2	2307	PASS
441	442	0.01	24	16.2	11217	PASS
442	198	50	100	65.0	69250	PASS
443	442	15	24	19.1	13244	PASS