


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012417\
 Data File : BF092437.D
 Acq On : 24 Jan 2017 19:05
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 24 13:48:07 2017

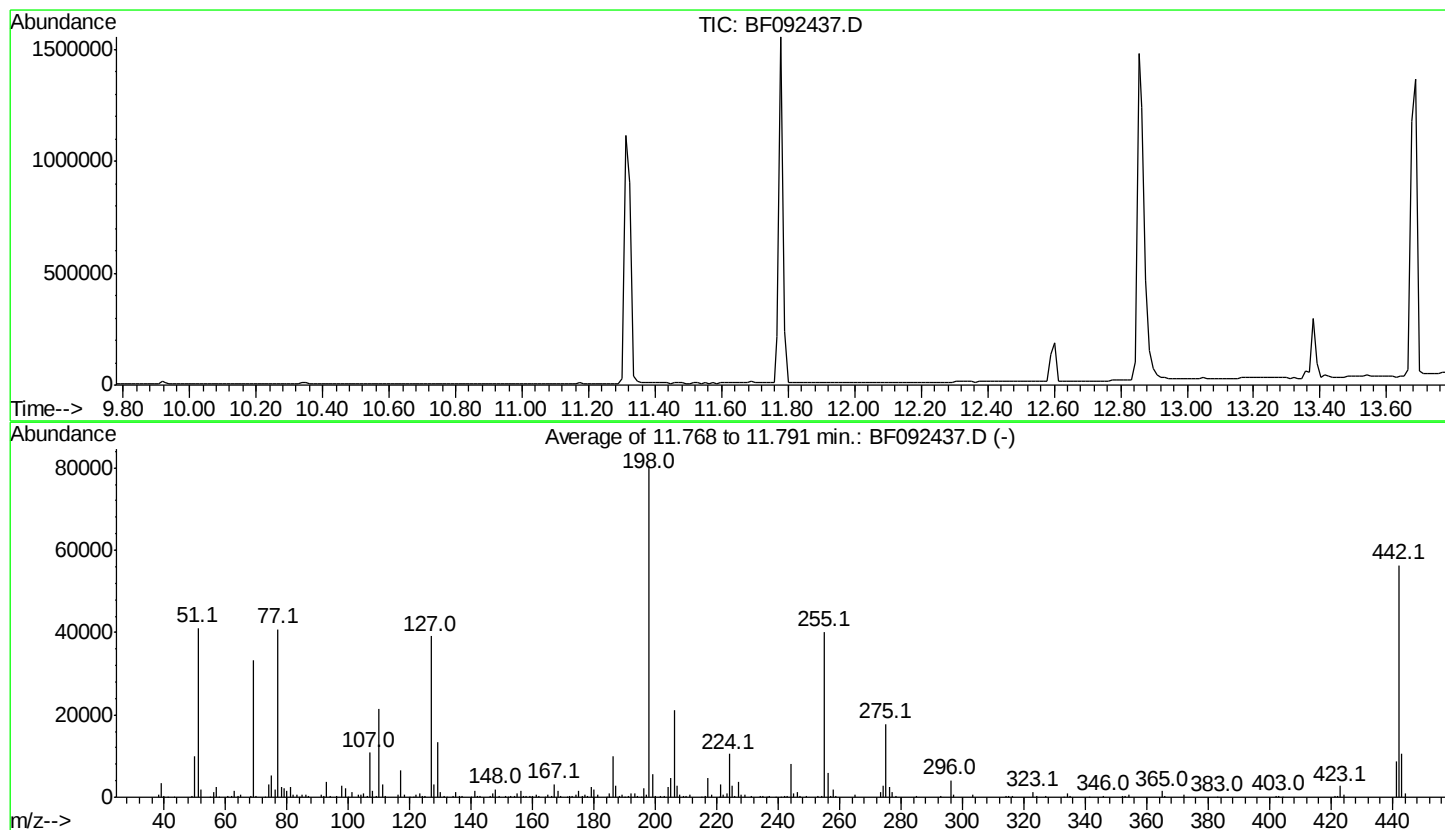

AutoFind: Scans 847, 848, 849; Background Corrected with Scan 844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.0	41111	PASS
68	69	0.00	2	1.3	445	PASS
69	198	0.00	100	41.3	33307	PASS
70	69	0.00	2	0.6	195	PASS
127	198	10	80	48.5	39087	PASS
197	198	0.00	2	0.9	710	PASS
198	198	100	100	100.0	80557	PASS
199	198	5	9	6.9	5584	PASS
275	198	10	60	22.2	17846	PASS
365	198	1	100	1.8	1489	PASS
441	442	0.01	24	15.5	8749	PASS
442	198	50	100	70.0	56363	PASS
443	442	15	24	19.0	10736	PASS