

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012418\
 Data File : BF102396.D
 Acq On : 24 Jan 2018 18:18
 Operator : SJ/JU
 Sample : J1249-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AB-3(0-2)

Quant Time: Jan 25 00:47:03 2018
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 23 00:43:41 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	129844	20.00	ng	0.00
21) Naphthalene-d8	8.00	136	543892	20.00	ng	0.00
38) Acenaphthene-d10	9.75	164	242953	20.00	ng	0.00
63) Phenanthrene-d10	11.23	188	395679	20.00	ng	0.00
75) Chrysene-d12	13.87	240	256159	20.00	ng	0.00
86) Perylene-d12	15.30	264	243188	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	932491	108.89	ng	0.00
7) Phenol-d6	6.36	99	1145957	111.00	ng	0.00
23) Nitrobenzene-d5	7.29	82	720247	76.10	ng	0.00
41) 2,4,6-Tribromophenol	10.54	330	197628	82.09	ng	0.00
44) 2-Fluorobiphenyl	9.07	172	1096355	66.35	ng	0.00
78) Terphenyl-d14	12.82	244	749498	65.96	ng	0.00
Target Compounds						
10) Phenol	6.37	94	62559	5.550	ng	92
49) Dimethylphthalate	9.47	163	131830	6.565	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012418\
Data File : BF102396.D
Acq On : 24 Jan 2018 18:18
Operator : SJ/JU
Sample : J1249-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AB-3(0-2)

Quant Time: Jan 25 00:47:03 2018
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 00:43:41 2018
Response via : Initial Calibration

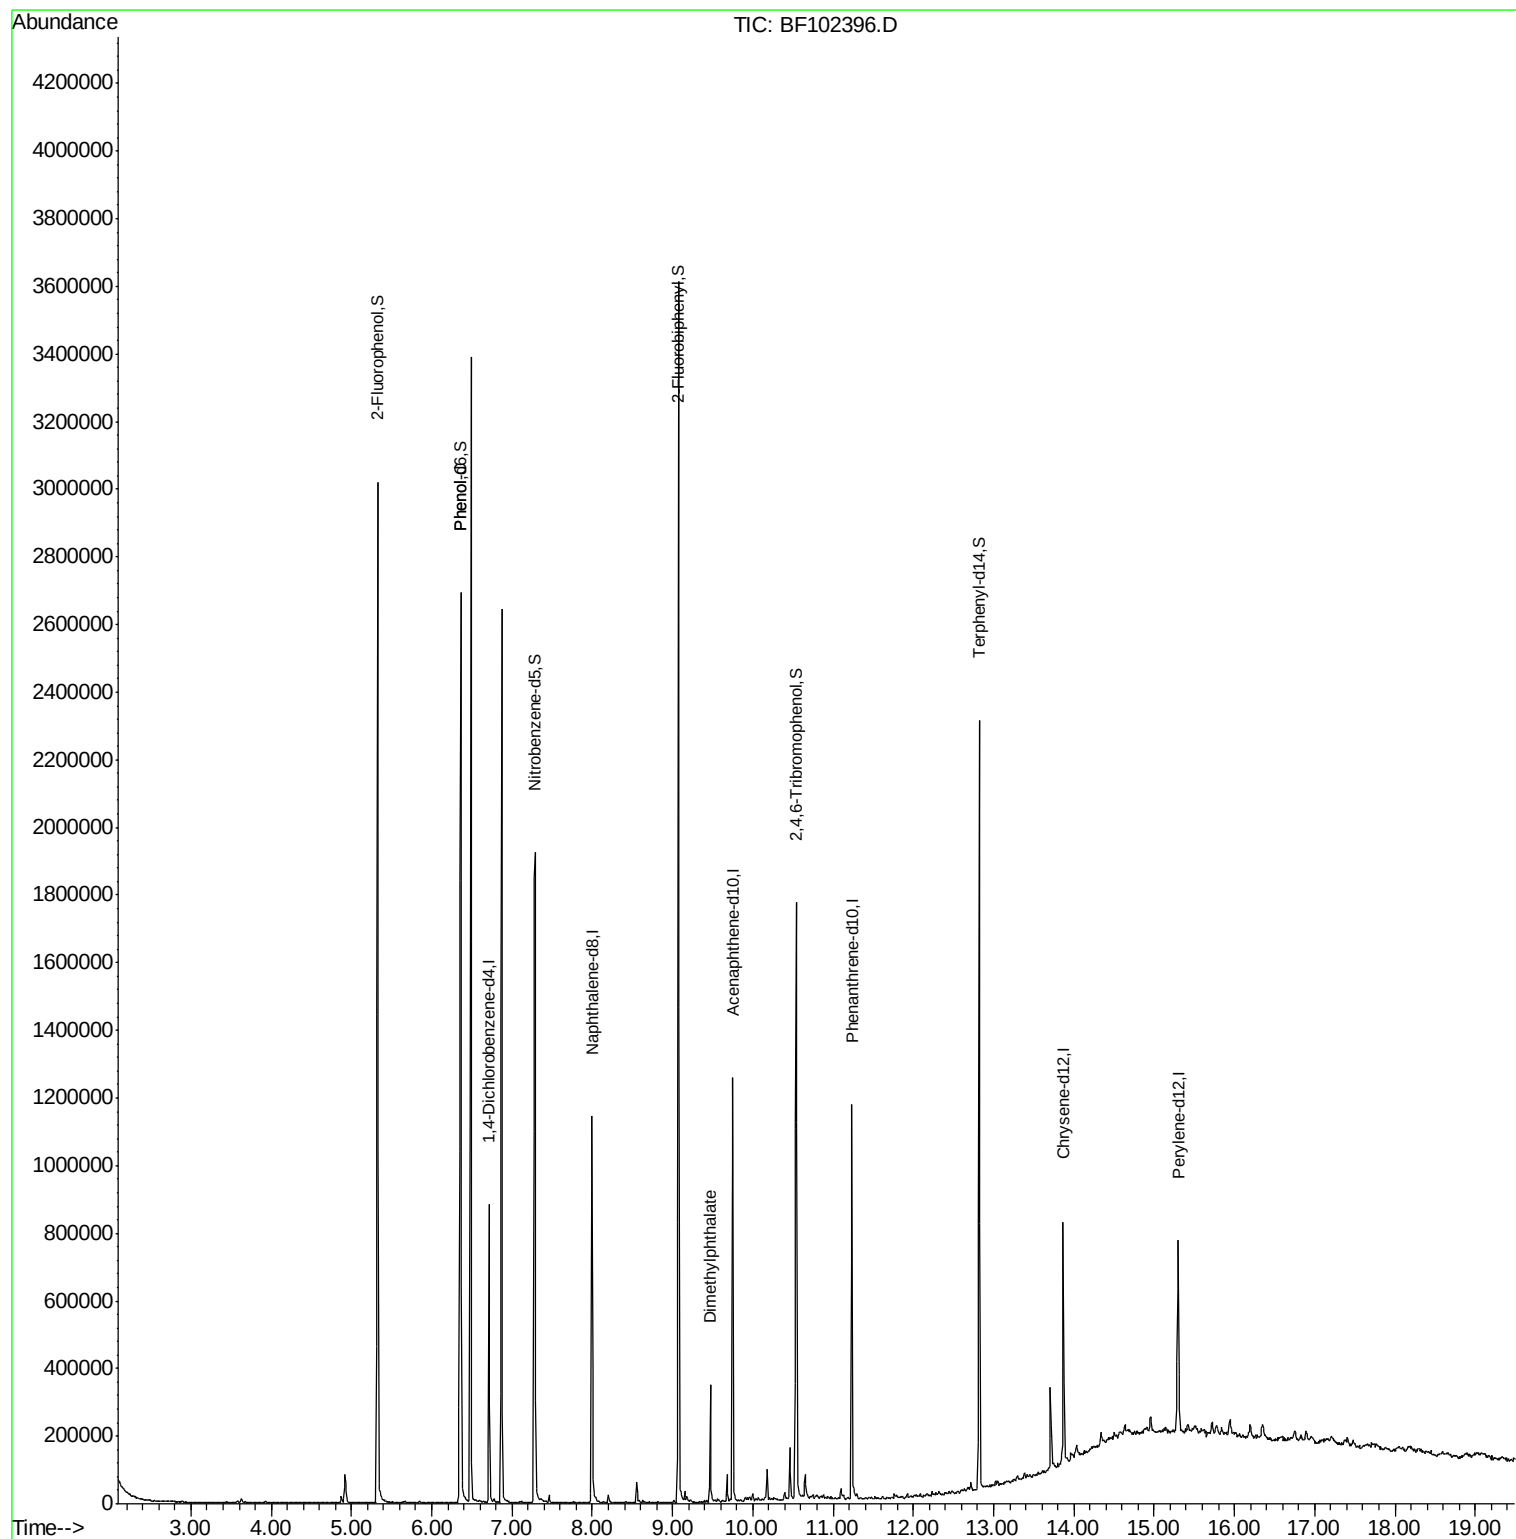

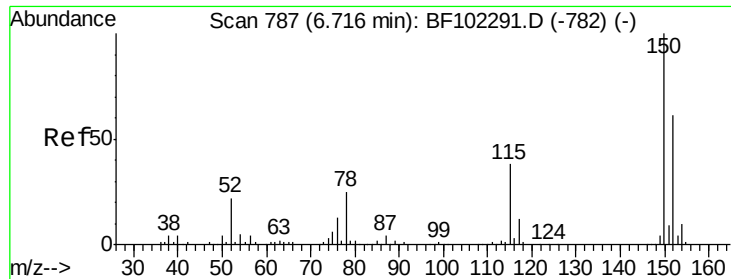


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.72 min Scan# 787
Delta R.T. -0.00 min
Lab File: BF102396.D
Acq: 24 Jan 2018 18:18

Instrument :
BNA_F
ClientSampleId :
AB-3(0-2)

Tgt Ion:152 Resp: 129844
Ion Ratio Lower Upper
152 100
150 156.5 124.6 186.8
115 62.0 50.1 75.1

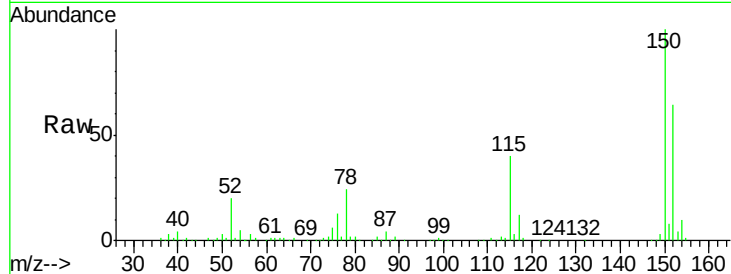


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

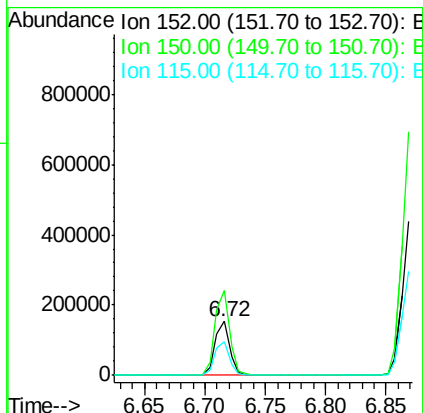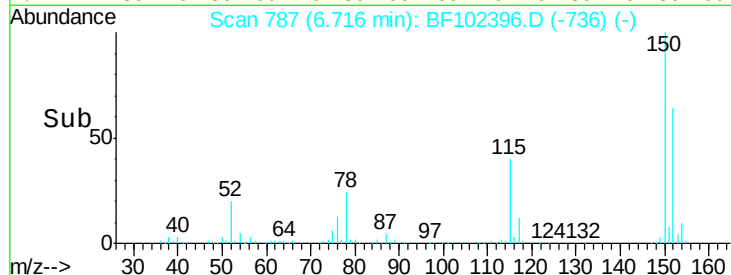



#5


2-Fluorophenol
Concen: 108.892 ng
RT: 5.33 min Scan# 551
Delta R.T. 0.01 min
Lab File: BF102396.D
Acq: 24 Jan 2018 18:18

Tgt Ion:112 Resp: 932491
Ion Ratio Lower Upper
112 100
64 58.7 47.9 71.9
63 30.0 23.7 35.5

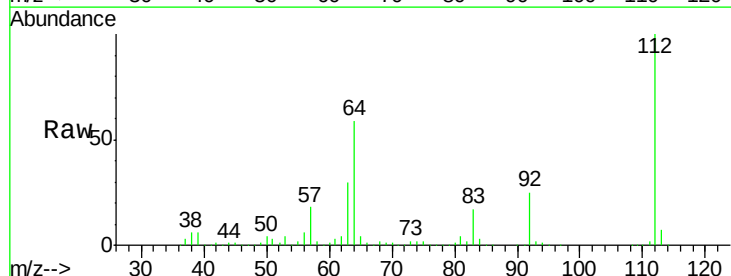

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

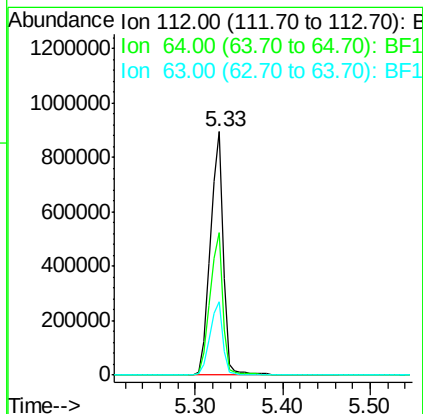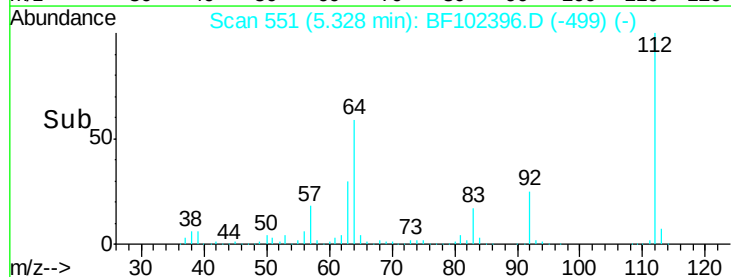

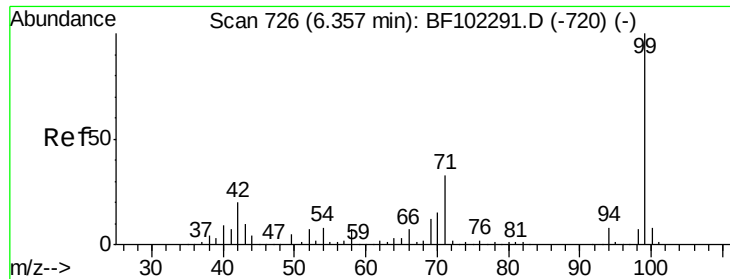

#7

Phenol-d6

Concen: 110.999 ng

RT: 6.36 min Scan# 727

Delta R.T. 0.01 min

Lab File: BF102396.D

Acq: 24 Jan 2018 18:18

Instrument :

BNA_F

ClientSampleId :

AB-3(0-2)


Tgt Ion: 99 Resp: 1145957

Ion Ratio Lower Upper




99 100

42 18.2 14.5 21.7

71 32.2 25.4 38.0

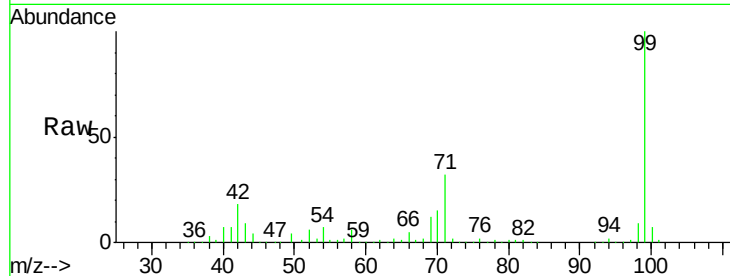

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

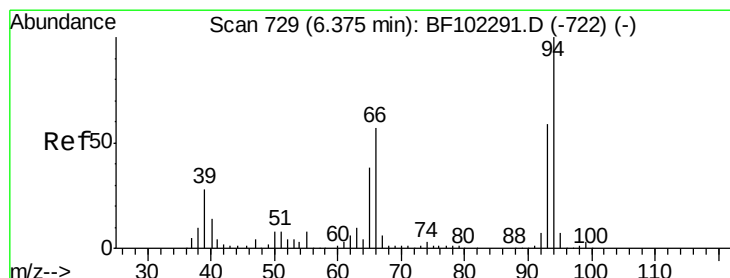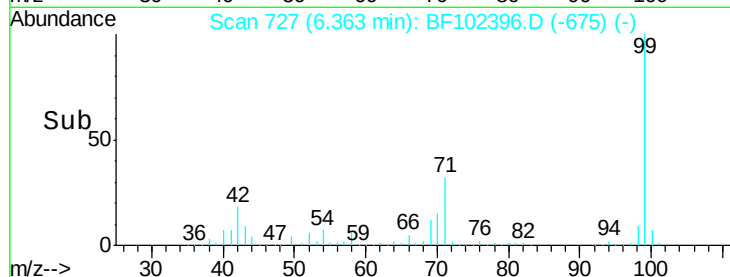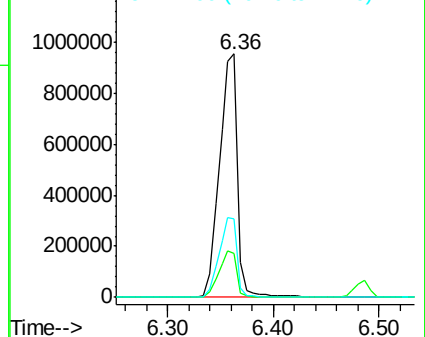

#10

Phenol

Concen: 5.550 ng

RT: 6.37 min Scan# 728

Delta R.T. -0.01 min

Lab File: BF102396.D

Acq: 24 Jan 2018 18:18


Tgt Ion: 94 Resp: 62559

Ion Ratio Lower Upper



94 100


65 26.9 7.9 47.9

66 43.3 16.2 56.2

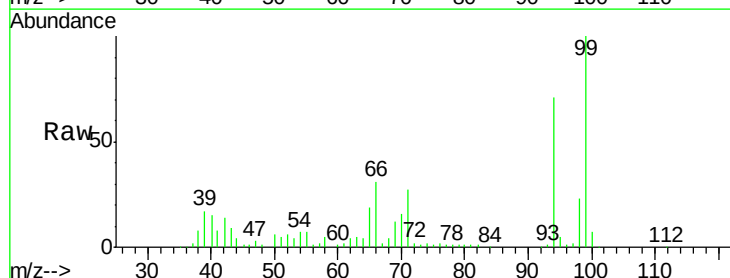

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

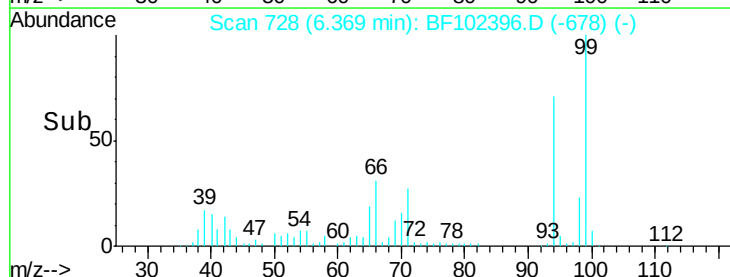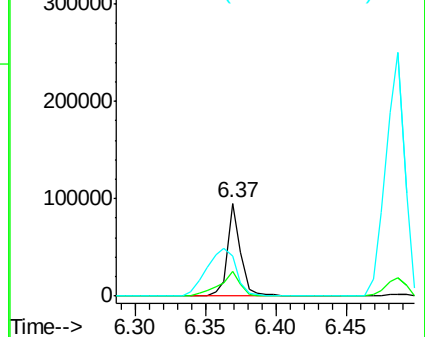


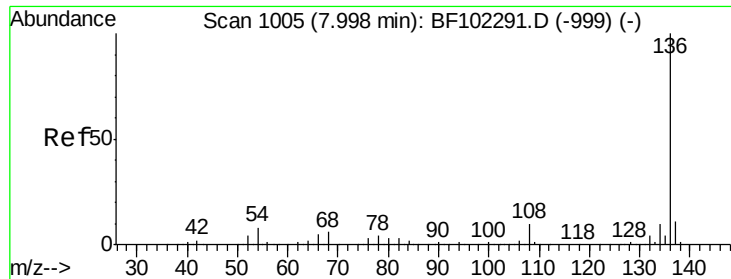




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.00 min Scan# 1005
Delta R.T. -0.00 min
Lab File: BF102396.D
Acq: 24 Jan 2018 18:18

Instrument :
BNA_F
ClientSampleId :
AB-3(0-2)

Tgt Ion: 136 Resp: 543892
Ion Ratio Lower Upper
136 100
137 11.1 8.9 13.3
54 7.7 6.6 9.8
68 5.3 5.0 7.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

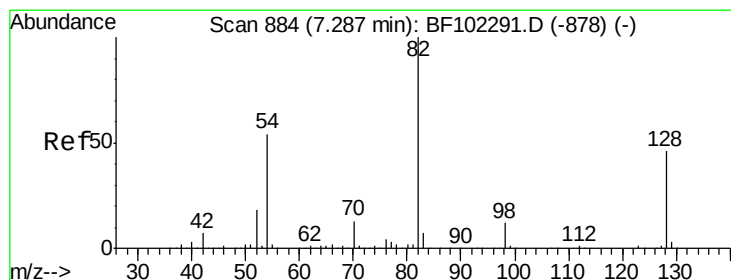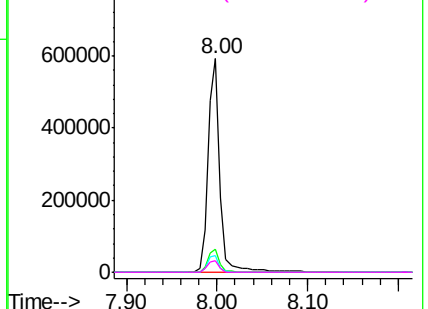
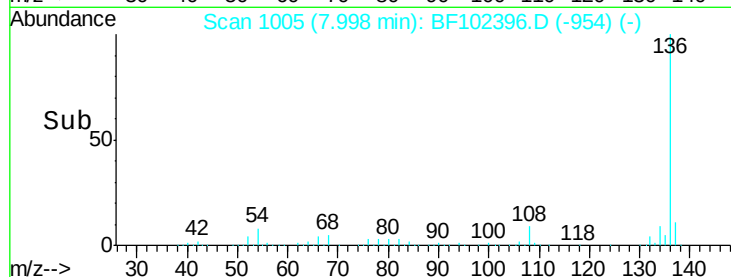



#23
Nitrobenzene-d5
Concen: 76.100 ng
RT: 7.29 min Scan# 884
Delta R.T. -0.00 min
Lab File: BF102396.D
Acq: 24 Jan 2018 18:18

Tgt Ion: 82 Resp: 720247
Ion Ratio Lower Upper
82 100
128 49.1 36.1 54.1
54 51.1 41.4 62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

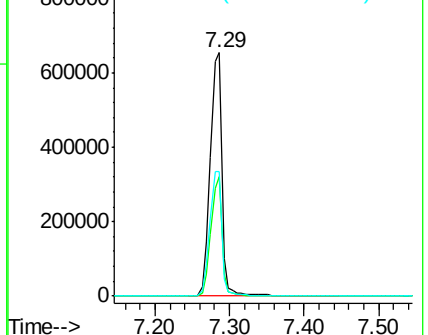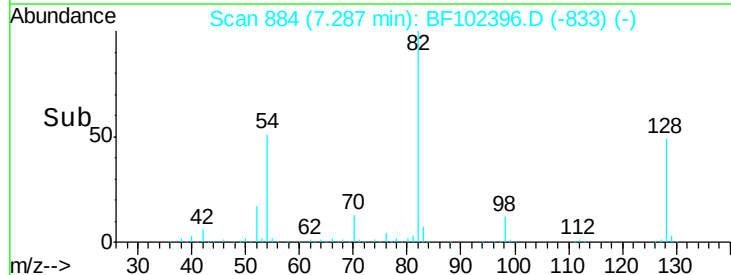


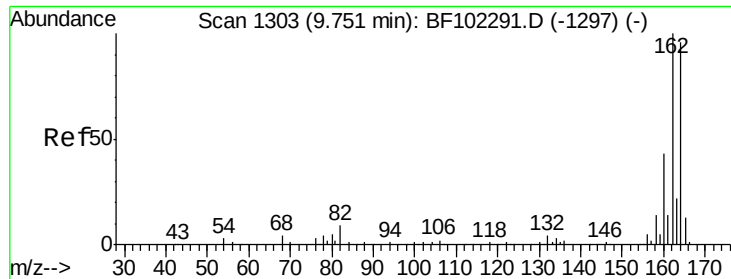




#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.75 min Scan# 1303
 Delta R.T. -0.00 min
 Lab File: BF102396.D
 Acq: 24 Jan 2018 18:18

Instrument :
 BNA_F
 ClientSampleId :
 AB-3(0-2)

Tgt Ion:164 Resp: 242953
 Ion Ratio Lower Upper
 164 100
 162 105.7 86.1 129.1
 160 45.5 38.3 57.5




Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

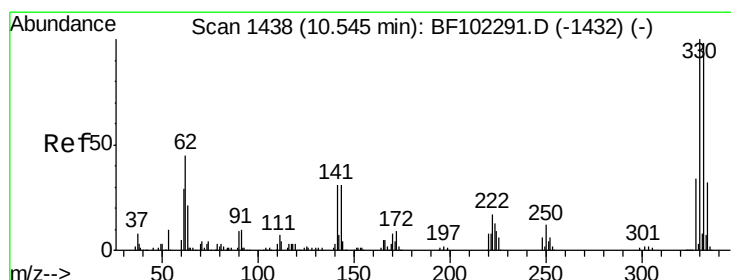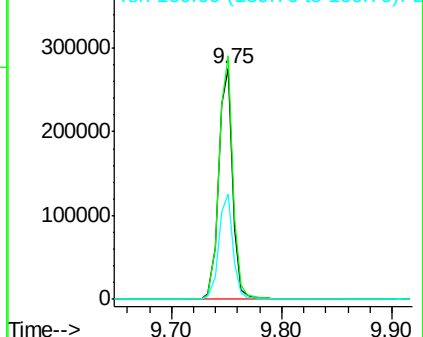
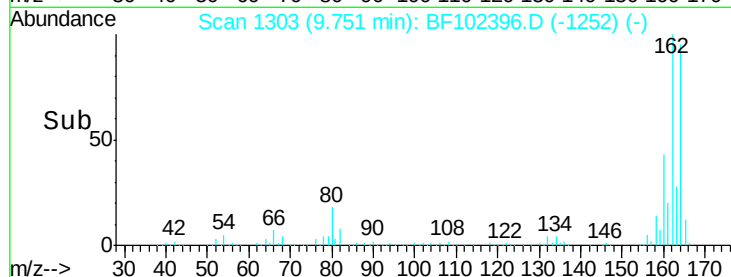



#41
 2,4,6-Tribromophenol
 Concen: 82.095 ng
 RT: 10.54 min Scan# 1437
 Delta R.T. -0.01 min
 Lab File: BF102396.D
 Acq: 24 Jan 2018 18:18

Tgt Ion:330 Resp: 197628
 Ion Ratio Lower Upper
 330 100
 332 96.6 77.0 115.6
 141 39.7 29.9 44.9



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



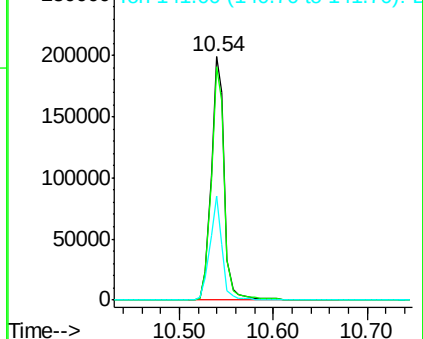
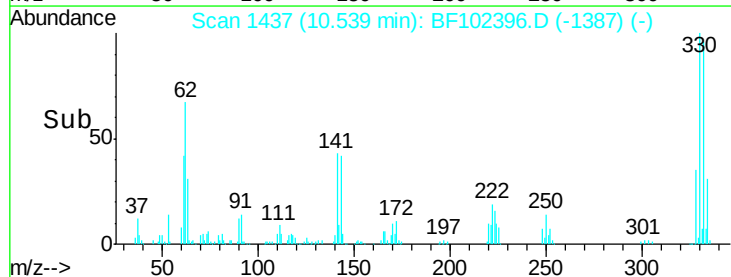


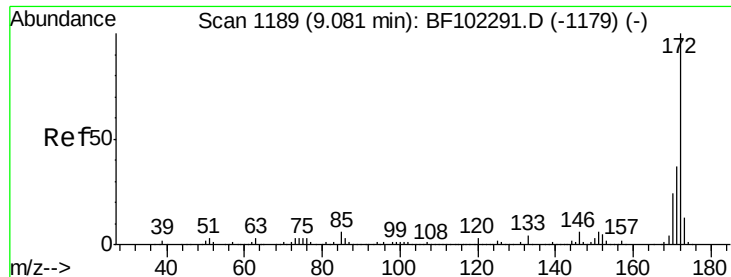

#44
2-Fluorobiphenyl
Concen: 66.351 ng
RT: 9.07 min Scan# 1188
Delta R.T. -0.01 min
Lab File: BF102396.D
Acq: 24 Jan 2018 18:18




Instrument :
BNA_F
ClientSampleId :
AB-3(0-2)


Tgt Ion:172 Resp: 1096355
Ion Ratio Lower Upper
172 100
171 35.7 29.7 44.5
170 23.8 19.6 29.4

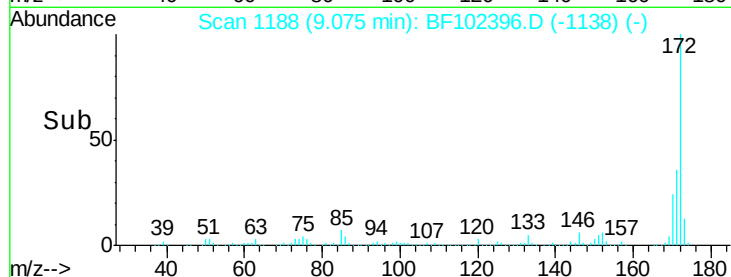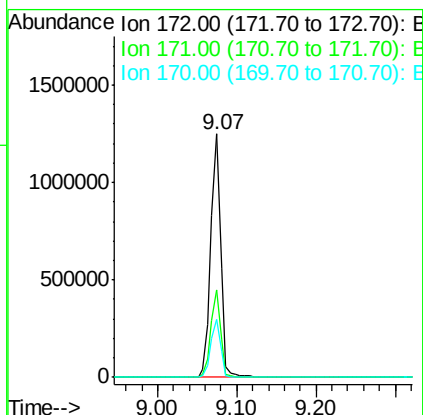

#49
Dimethylphthalate
Concen: 6.565 ng
RT: 9.47 min Scan# 1255
Delta R.T. -0.01 min
Lab File: BF102396.D
Acq: 24 Jan 2018 18:18

Tgt Ion:163 Resp: 131830
Ion Ratio Lower Upper
163 100
194 3.5 2.7 4.1
164 9.9 8.2 12.2

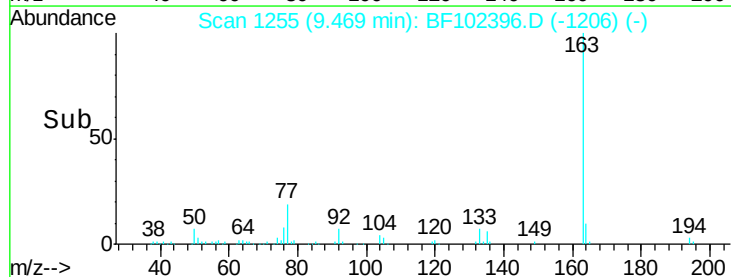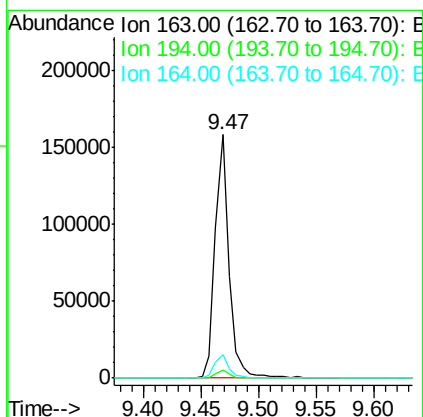

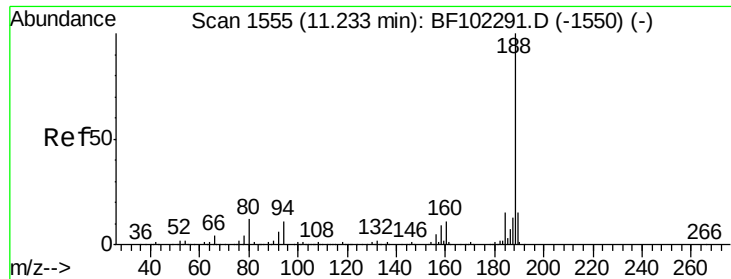

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.23 min Scan# 1555

Delta R.T. -0.00 min

Lab File: BF102396.D

Acq: 24 Jan 2018 18:18

Instrument :

BNA_F

ClientSampleId :

AB-3(0-2)


Tgt Ion:188 Resp: 395679

Ion Ratio Lower Upper

188 100

94 10.6 8.5 12.7




80 11.5 9.2 13.8



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

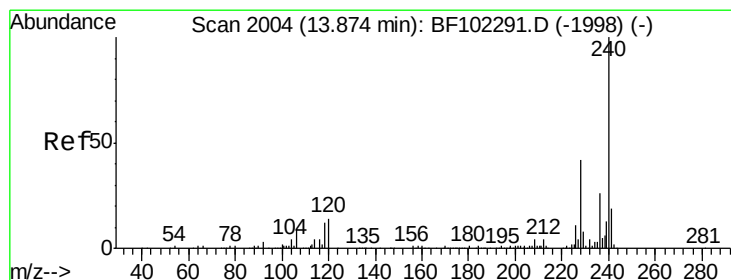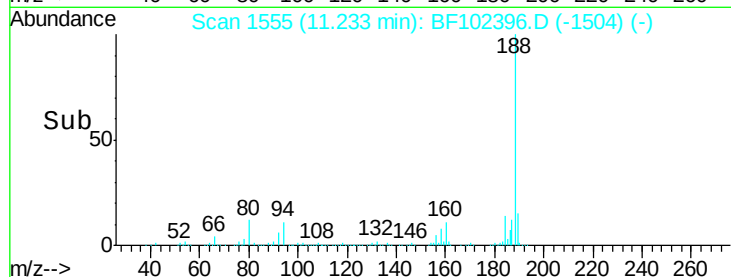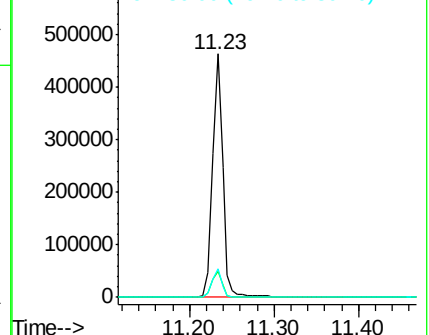

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.87 min Scan# 2004

Delta R.T. -0.00 min

Lab File: BF102396.D

Acq: 24 Jan 2018 18:18


Tgt Ion:240 Resp: 256159

Ion Ratio Lower Upper

240 100

120 11.7 9.5 14.3



236 25.7 20.7 31.1

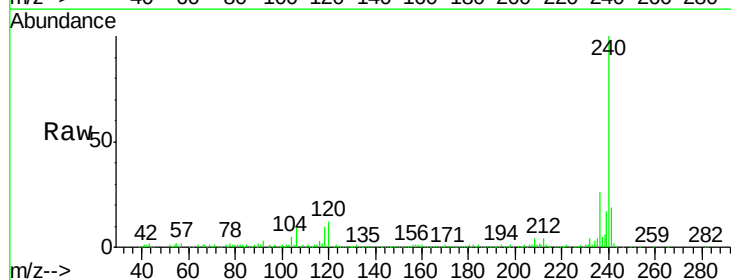


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



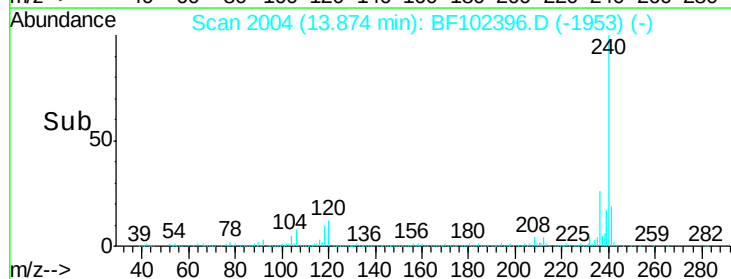
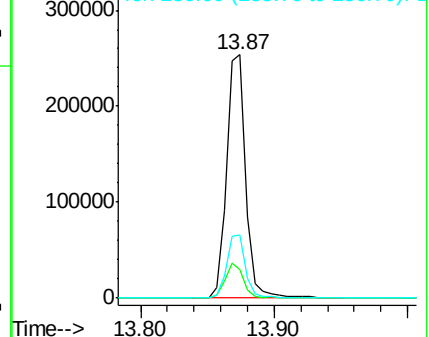


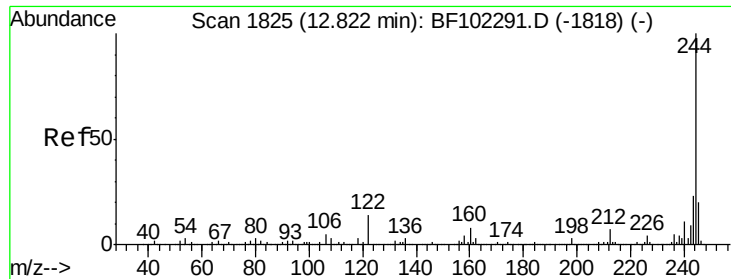

#78
 Terphenyl-d14
 Concen: 65.961 ng
 RT: 12.82 min Scan# 1825
 Delta R.T. -0.00 min
 Lab File: BF102396.D
 Acq: 24 Jan 2018 18:18

Instrument :
 BNA_F
 ClientSampleId :
 AB-3(0-2)

Tgt Ion:244 Resp: 749498
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.4 8.0
 122 12.9 11.0 16.4

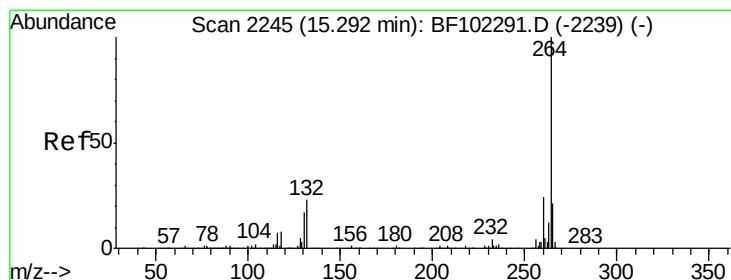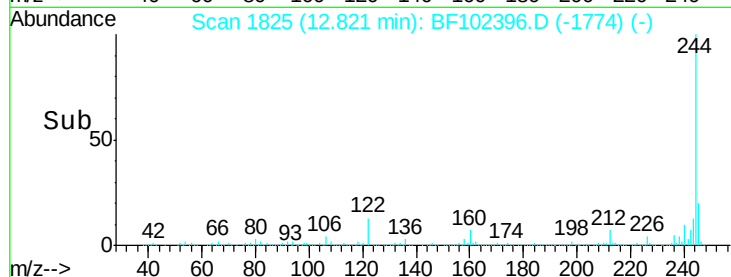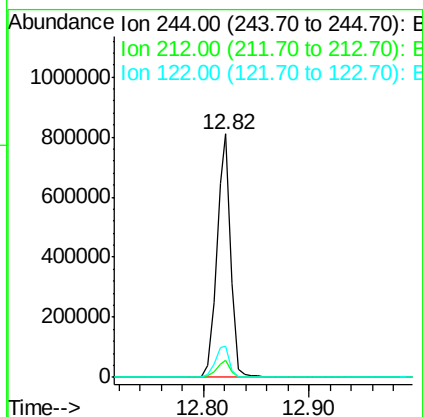

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.30 min Scan# 2246
 Delta R.T. 0.01 min
 Lab File: BF102396.D
 Acq: 24 Jan 2018 18:18

Tgt Ion:264 Resp: 243188
 Ion Ratio Lower Upper
 264 100
 260 24.7 19.2 28.8
 265 21.7 17.5 26.3

