


Data Path : Z:\HPCHEM1\BNA_F\Data\BF012418\
 Data File : BF102388.D
 Acq On : 24 Jan 2018 14:36
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 23 00:43:41 2018

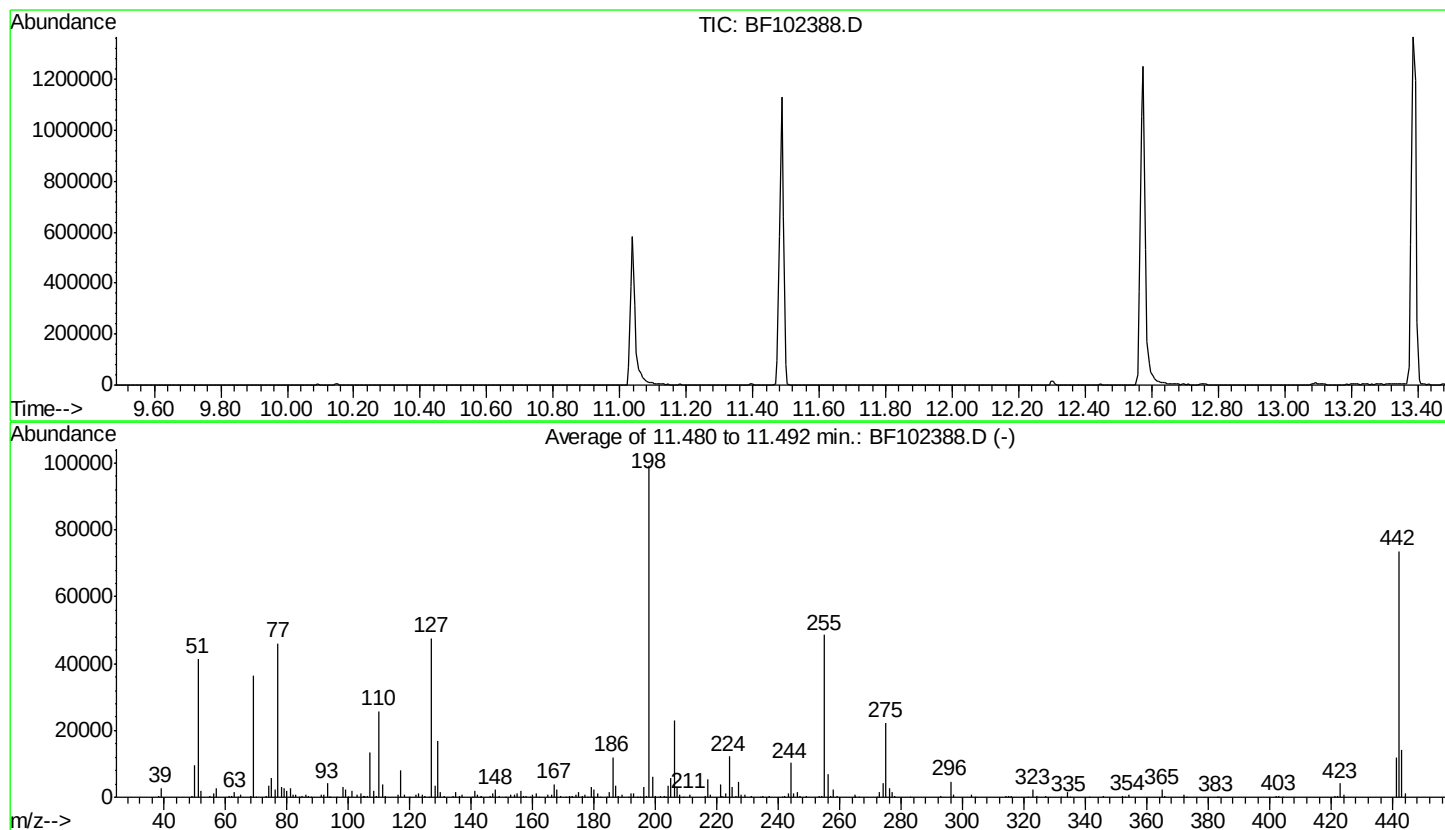

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	41573	PASS
68	69	0.00	2	1.5	529	PASS
69	198	0.00	100	36.7	36400	PASS
70	69	0.00	2	0.4	146	PASS
127	198	10	80	48.0	47677	PASS
197	198	0.00	2	0.2	224	PASS
198	198	100	100	100.0	99264	PASS
199	198	5	9	6.1	6029	PASS
275	198	10	60	22.4	22229	PASS
365	198	1	100	2.3	2242	PASS
441	443	0.01	100	83.9	12027	PASS
442	198	50	100	74.1	73576	PASS
443	442	15	24	19.5	14337	PASS