
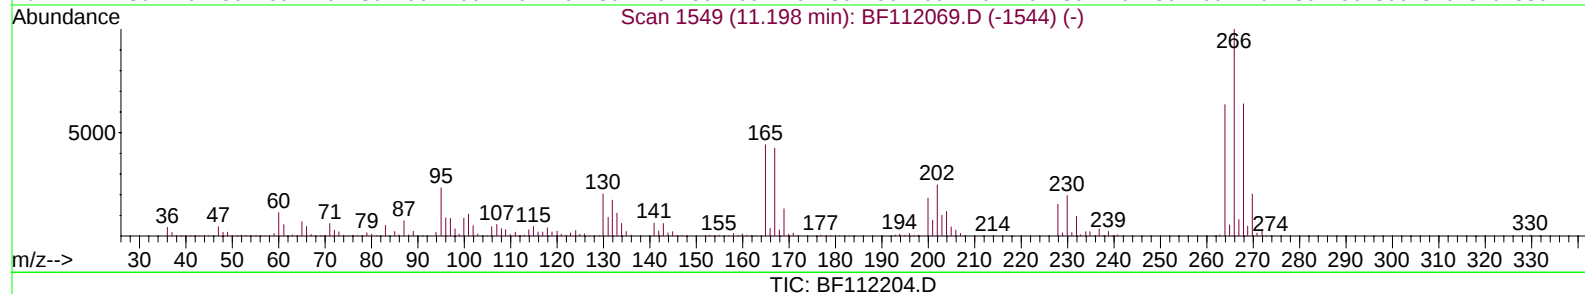
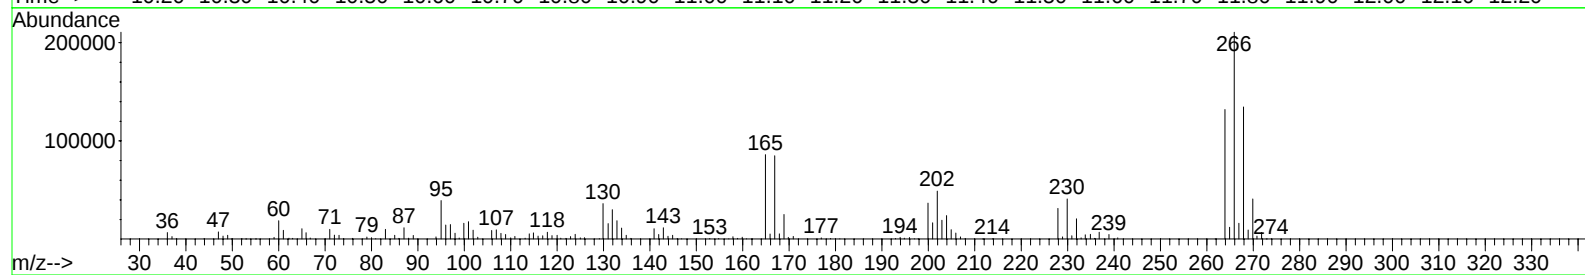


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012419\
Data File : BF112204.D
Acq On : 24 Jan 2019 12:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 15:47:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 19 01:02:12 2019
Response via : Initial Calibration

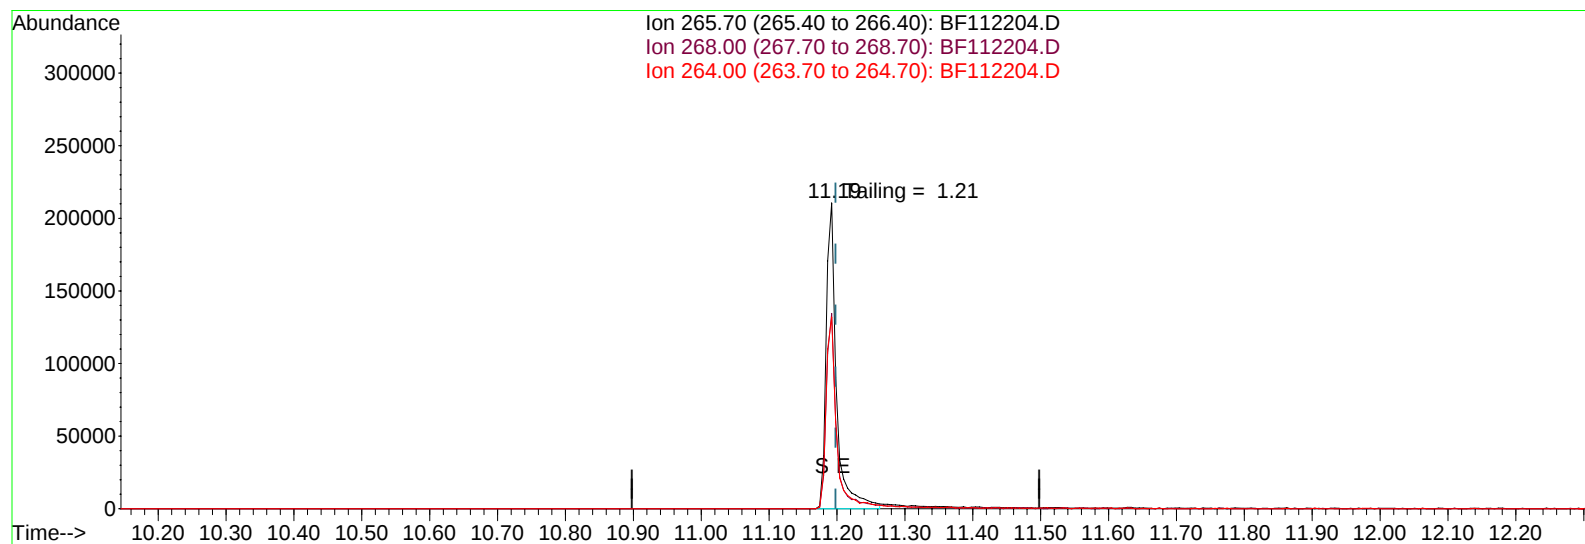

(70) Pentachlorophenol (C)




11.192min (-0.006) 31914.03ng

response 228806

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.89
264.00	63.60	62.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF012419\
Data File : BF112204.D
Acq On : 24 Jan 2019 12:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 15:47:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF011619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 19 01:02:12 2019
Response via : Initial Calibration

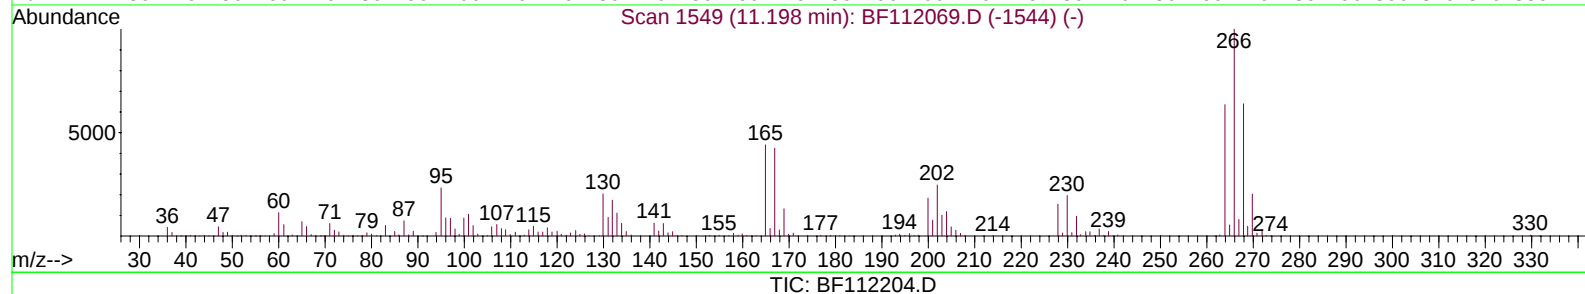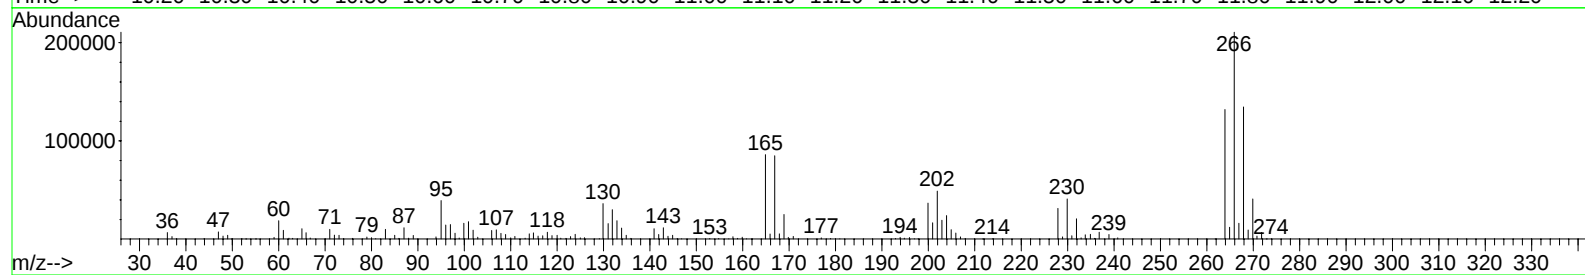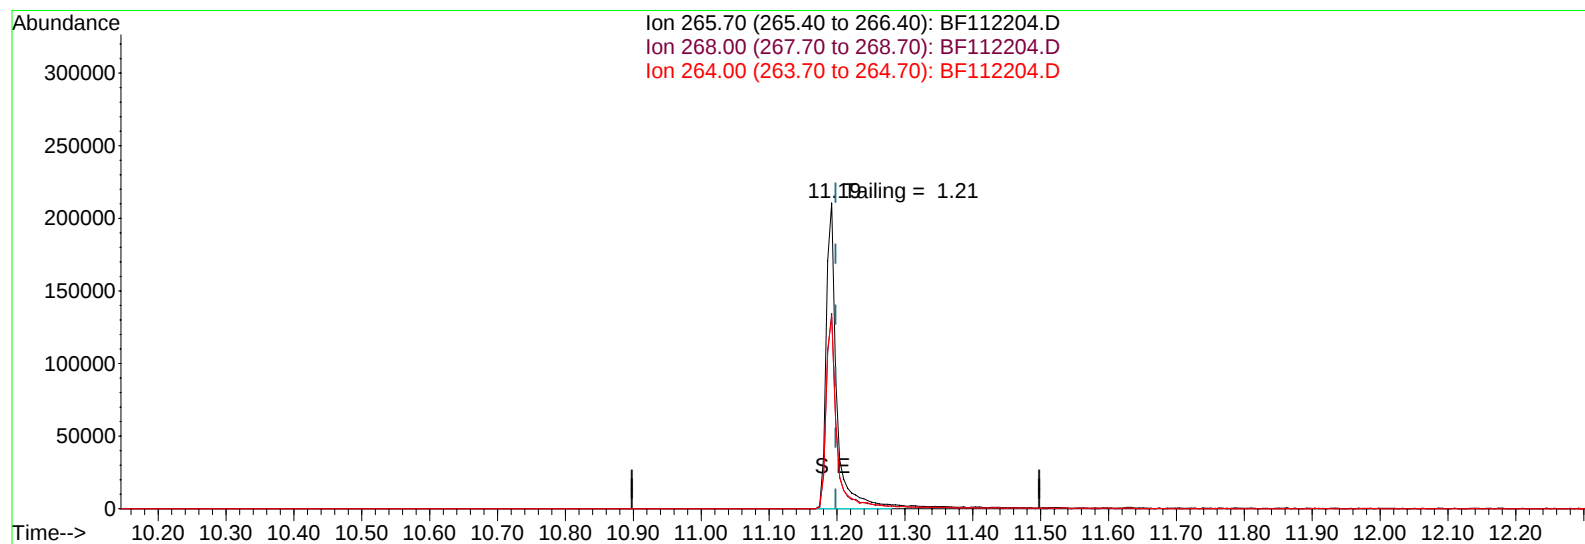

(70) Pentachlorophenol (C)

11.192min (-0.006) 31914.03ng

response 228806

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.89
264.00	63.60	62.67
0.00	0.00	0.00