


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012419\
 Data File : BF112204.D
 Acq On : 24 Jan 2019 12:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF011619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 19 01:02:12 2019

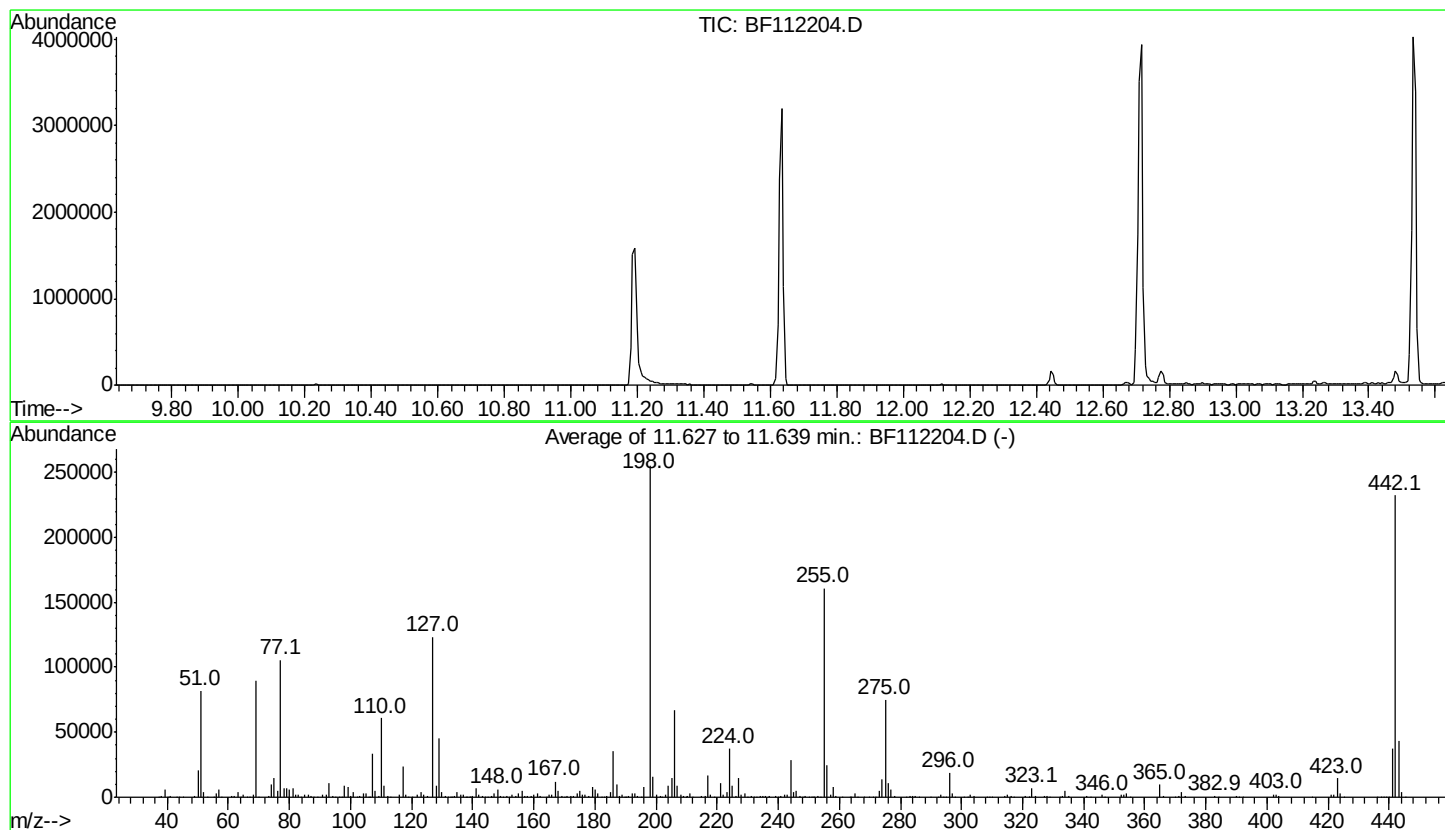

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	82261	PASS
68	69	0.00	2	1.9	1722	PASS
69	198	0.00	100	35.2	89810	PASS
70	69	0.00	2	0.5	409	PASS
127	198	10	80	48.3	123210	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	255144	PASS
199	198	5	9	6.3	16116	PASS
275	198	10	60	29.5	75146	PASS
365	198	1	100	3.9	9847	PASS
441	198	0.01	100	14.7	37448	PASS
442	198	50	100	91.0	232234	PASS
443	442	15	24	18.7	43517	PASS