


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012420\
 Data File : BF118681.D
 Acq On : 24 Jan 2020 12:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 27 01:13:13 2020

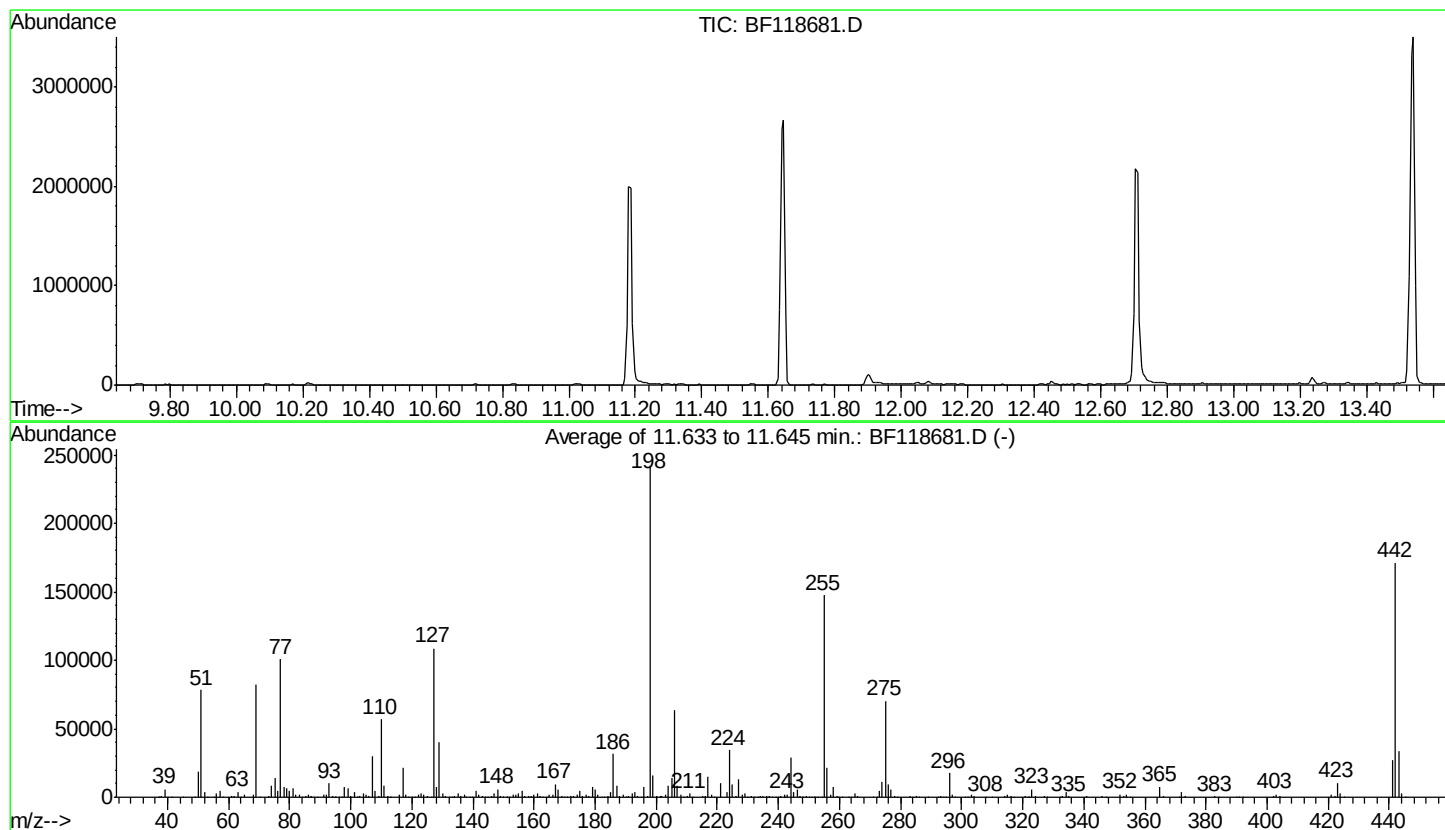

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	78114	PASS
68	69	0.00	2	1.9	1602	PASS
69	198	0.00	100	34.2	82725	PASS
70	69	0.00	2	0.5	440	PASS
127	198	10	80	44.8	108552	PASS
197	198	0.00	2	0.5	1318	PASS
198	198	100	100	100.0	242152	PASS
199	198	5	9	6.8	16354	PASS
275	198	10	60	29.0	70149	PASS
365	198	1	100	3.2	7693	PASS
441	198	0.01	100	11.1	26853	PASS
442	198	50	100	70.8	171477	PASS
443	442	15	24	19.8	33954	PASS