


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF012420\
 Data File : BF118705.D
 Acq On : 25 Jan 2020 00:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 27 01:13:13 2020

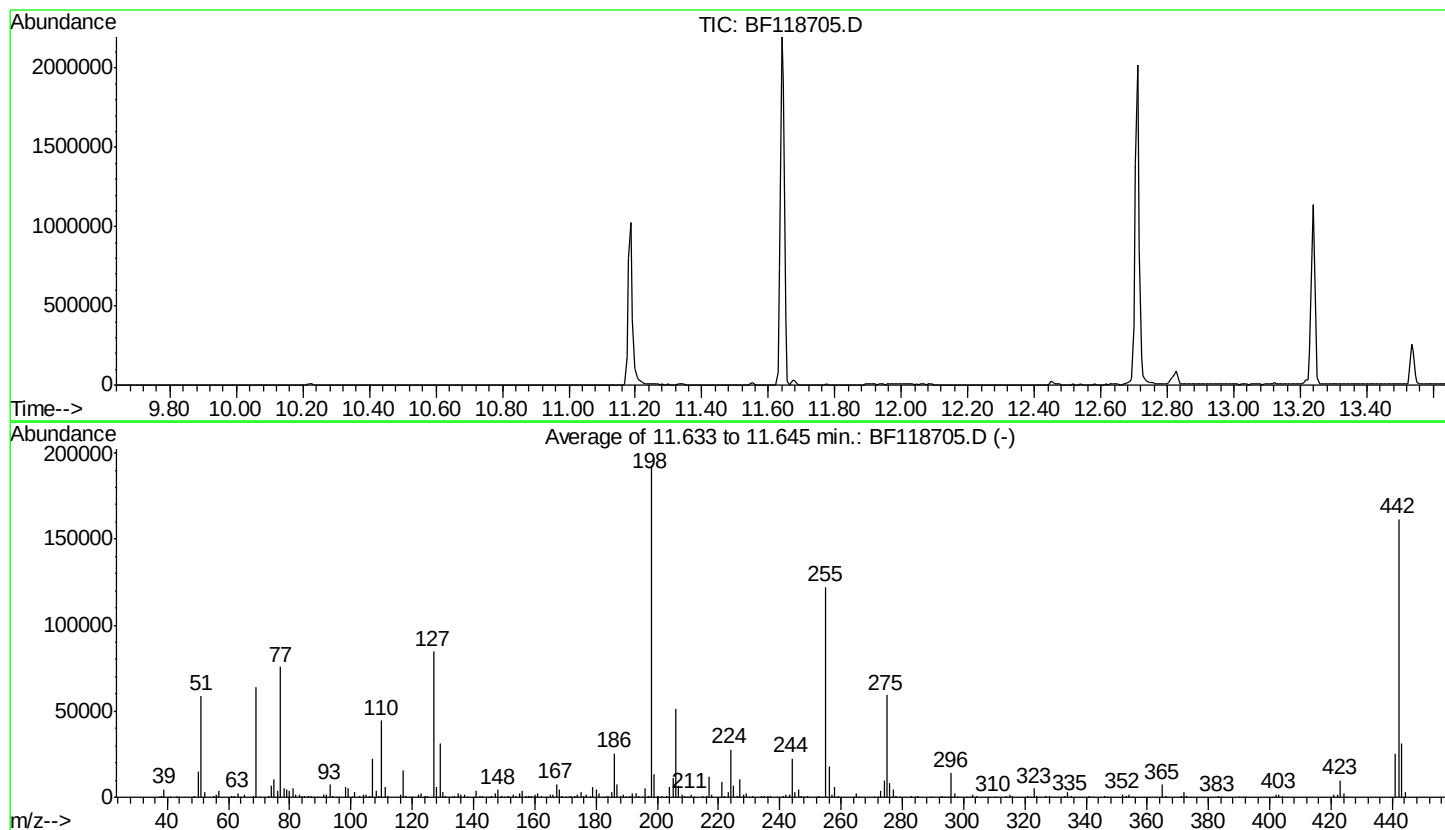

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	58818	PASS
68	69	0.00	2	1.3	861	PASS
69	198	0.00	100	33.2	63997	PASS
70	69	0.00	2	0.5	342	PASS
127	198	10	80	43.9	84664	PASS
197	198	0.00	2	0.2	438	PASS
198	198	100	100	100.0	192698	PASS
199	198	5	9	6.9	13371	PASS
275	198	10	60	30.8	59384	PASS
365	198	1	100	3.8	7238	PASS
441	198	0.01	100	13.0	25068	PASS
442	198	50	100	83.8	161429	PASS
443	442	15	24	19.5	31490	PASS