
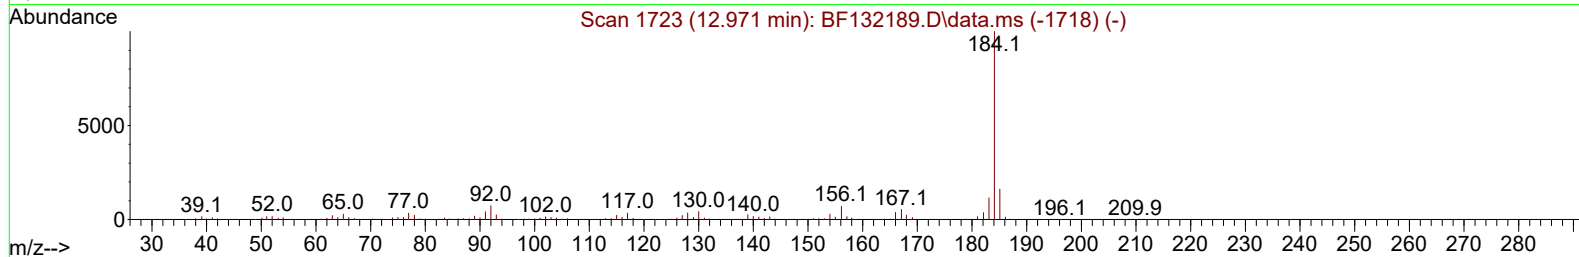
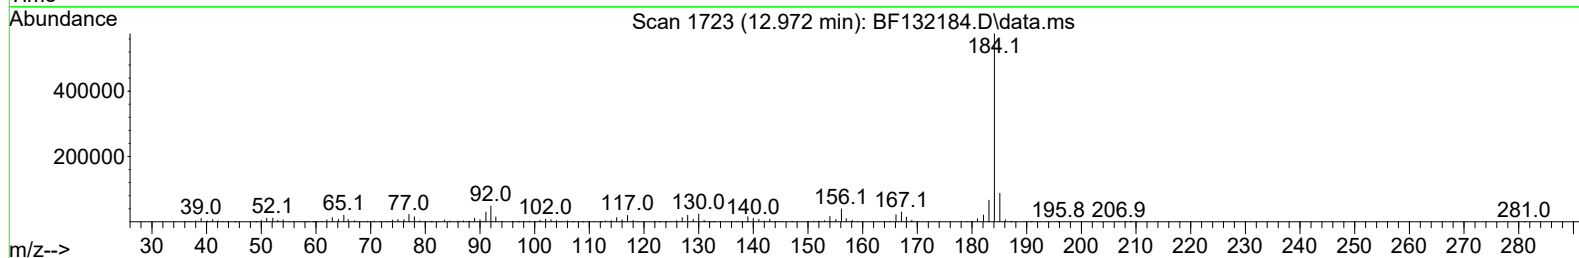


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012423\
 Data File : BF132184.D
 Acq On : 24 Jan 2023 09:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 06:05:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 02:09:50 2023
 Response via : Initial Calibration

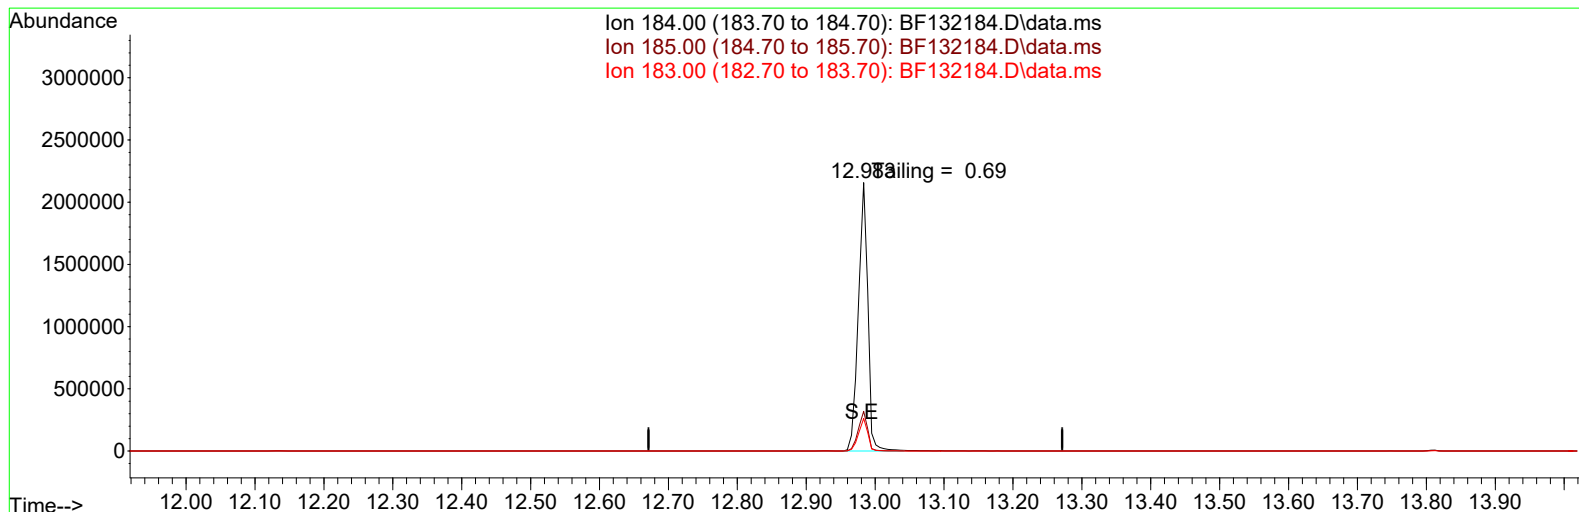

TIC: BF132184.D\data.ms

(77) Benzidine




12.971min (-12.971) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	16.20	0.00#
183.00	11.50	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012423\
 Data File : BF132184.D
 Acq On : 24 Jan 2023 09:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 06:05:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012423.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 02:09:50 2023
 Response via : Initial Calibration

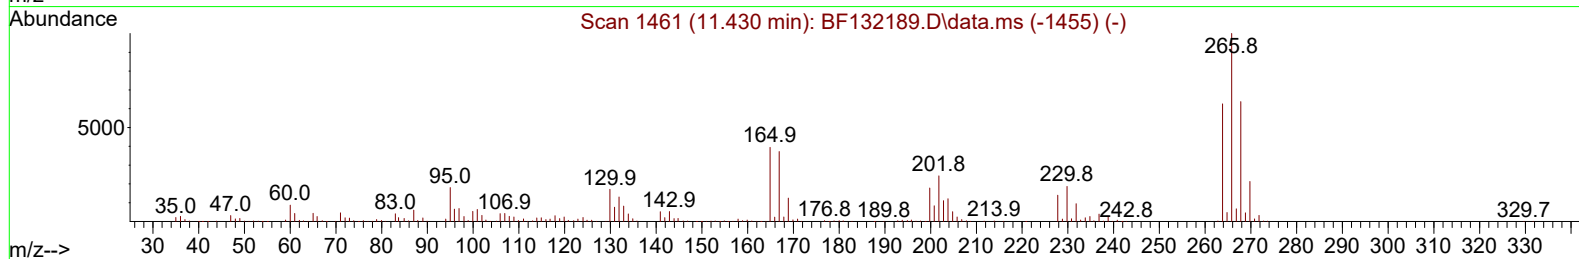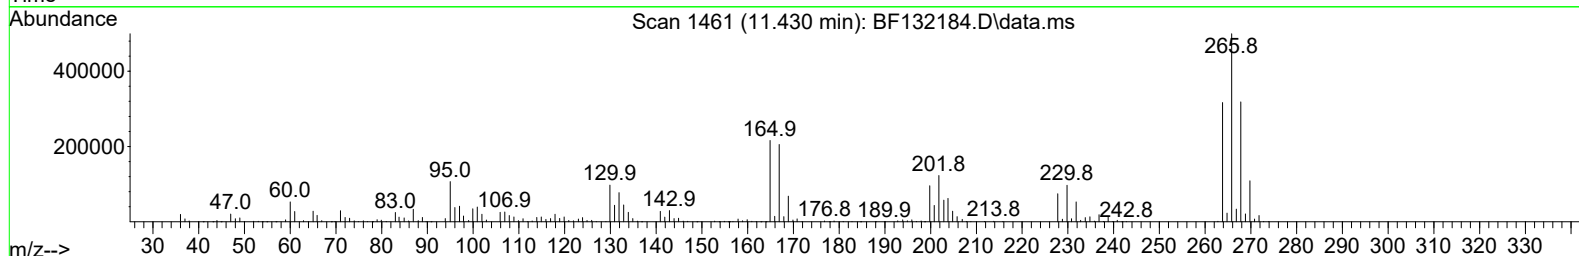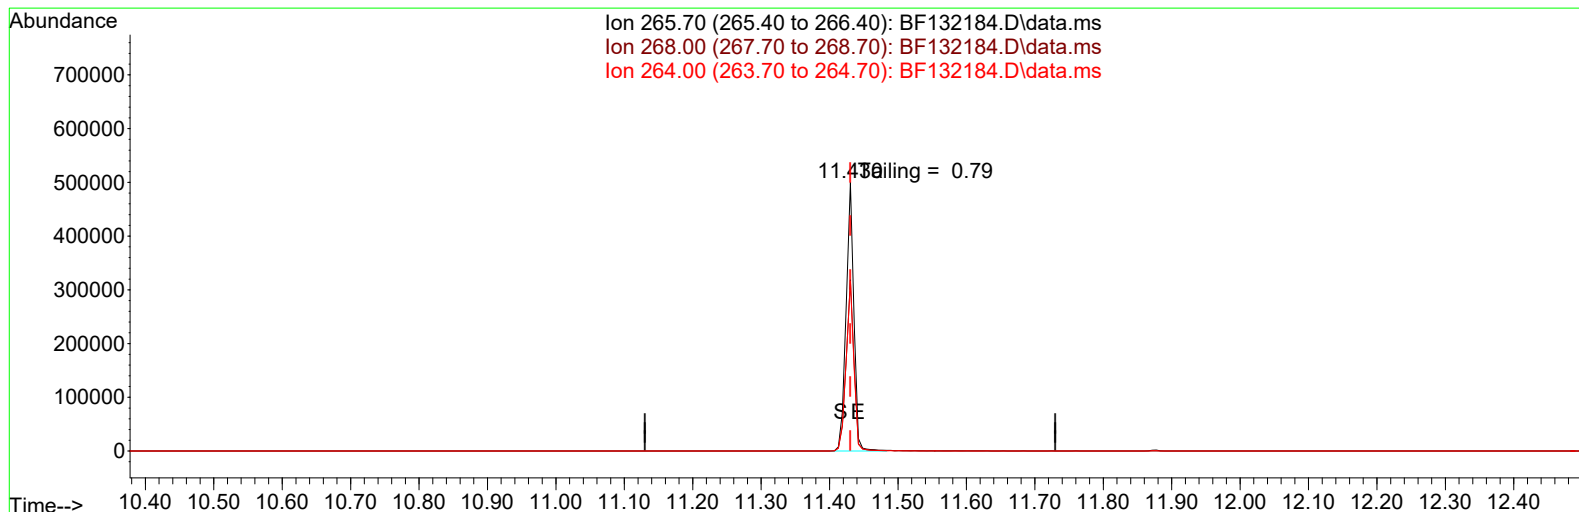

TIC: BF132184.D\data.ms

(70) Pentachlorophenol (C)

11.430min (+ 0.000) 357864.42 ng

response 398862

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.73
264.00	62.60	63.40
0.00	0.00	0.00