


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF012423\  
Data File : BF132184.D  
Acq On : 24 Jan 2023 09:25  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF012423.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Jan 25 02:09:50 2023

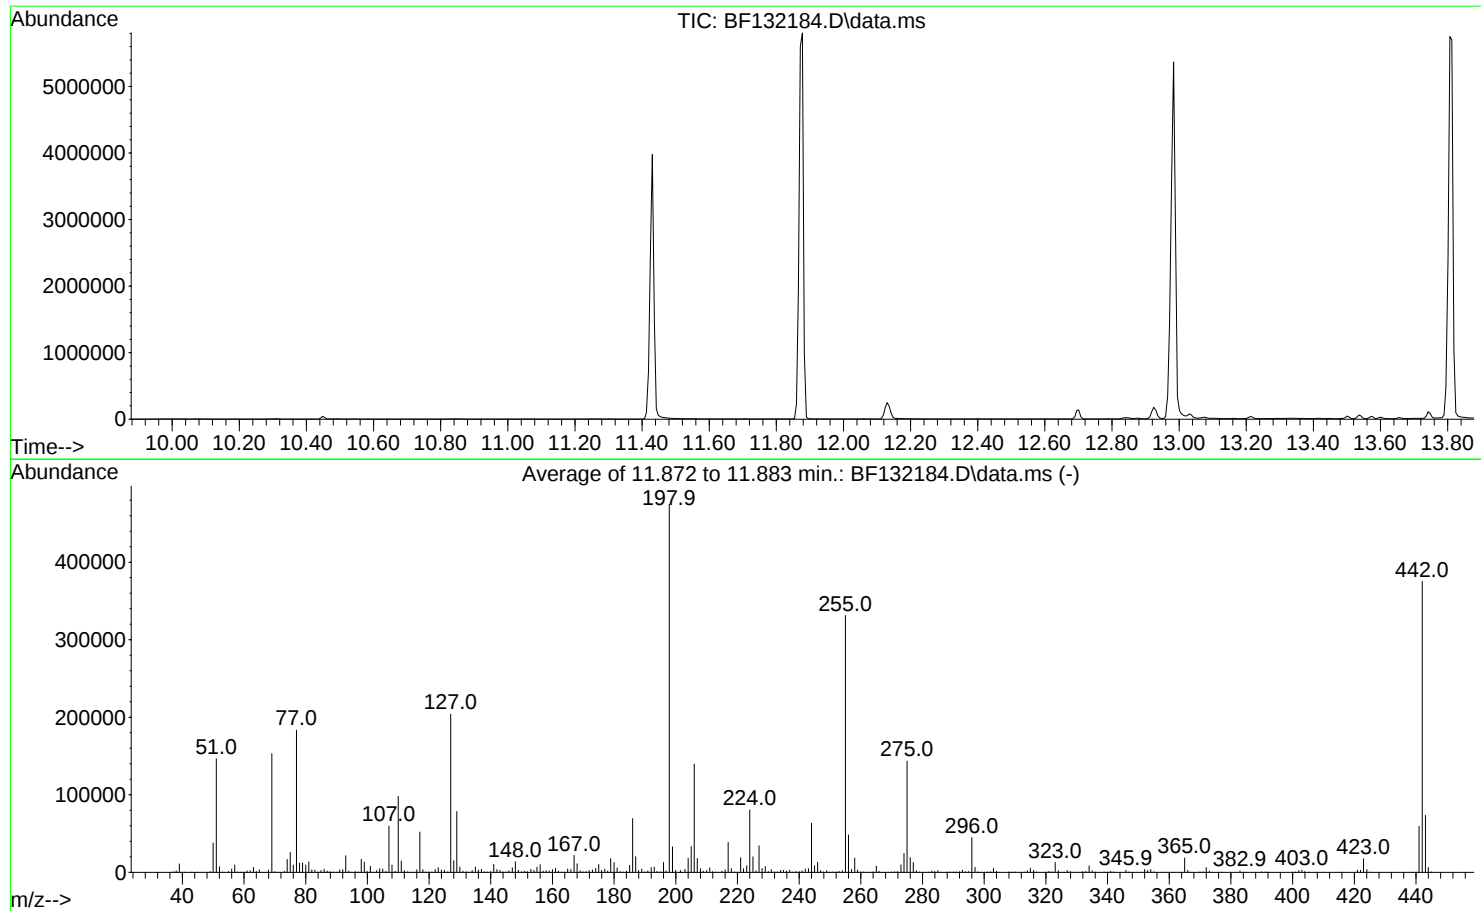




AutoFind: Scans 1536, 1537, 1538; Background Corrected with Scan 1530

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 30.8         | 146376     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 2727       | PASS                |
| 69             | 198             | 0.00            | 100             | 32.2         | 153019     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 932        | PASS                |
| 127            | 198             | 10              | 80              | 43.0         | 203824     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 1856       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 474528     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 32959      | PASS                |
| 275            | 198             | 10              | 60              | 30.2         | 143280     | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 18507      | PASS                |
| 441            | 198             | 0.01            | 100             | 12.5         | 59416      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 375125     | PASS                |
| 443            | 442             | 15              | 24              | 19.6         | 73373      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF012423\  
 Data File : BF132184.D  
 Acq On : 24 Jan 2023 09:25  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Jan 25 06:05:07 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF012423.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Jan 25 02:09:50 2023  
 Response via : Initial Calibration

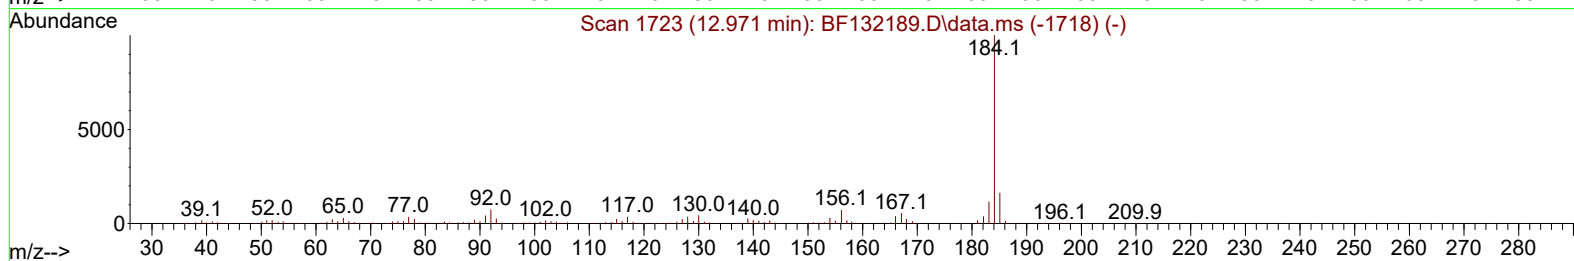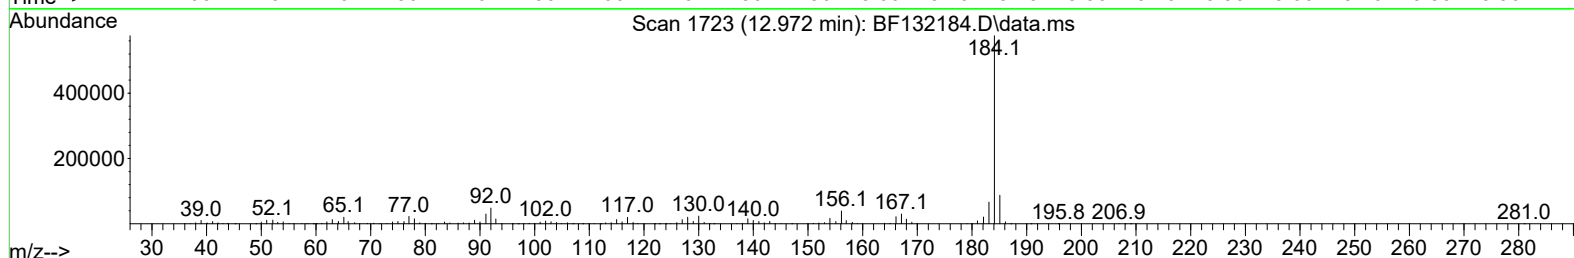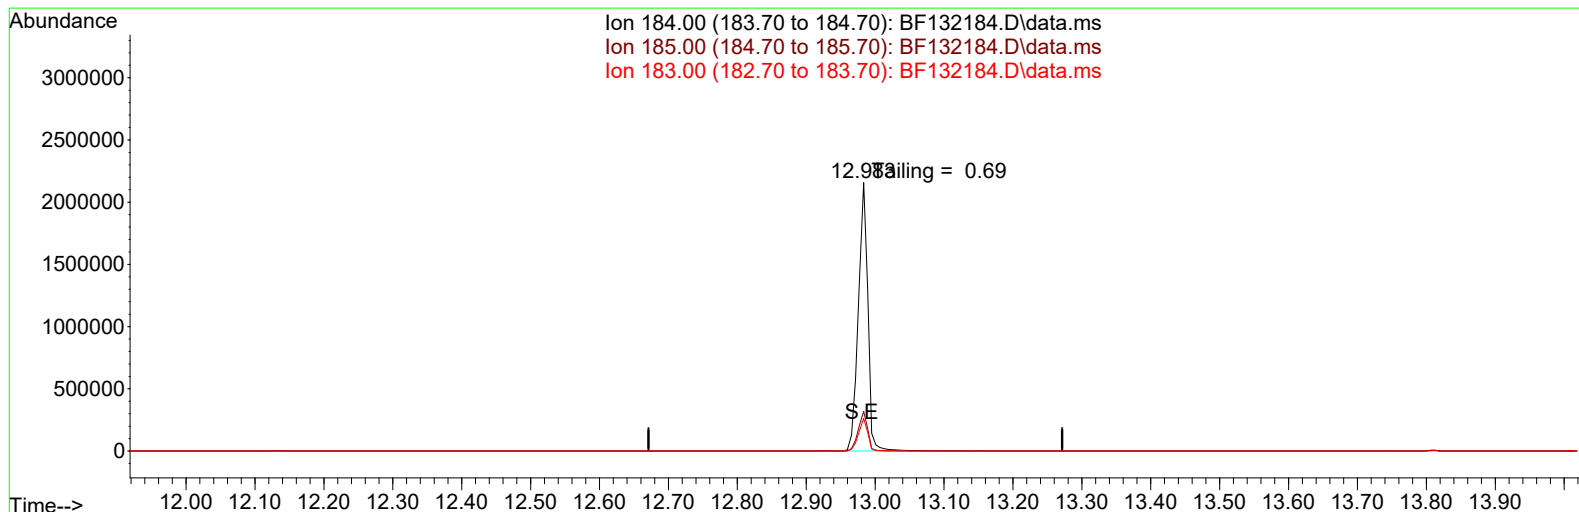

TIC: BF132184.D\data.ms

**(77) Benzidine**

12.971min (-12.971) 0.00 ng




response 0

| Ion    | Exp%   | Act%  |
|--------|--------|-------|
| 184.00 | 100.00 | 0.00  |
| 185.00 | 16.20  | 0.00# |
| 183.00 | 11.50  | 0.00# |
| 0.00   | 0.00   | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF012423\  
Data File : BF132184.D  
Acq On : 24 Jan 2023 09:25  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jan 25 06:05:07 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF012423.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jan 25 02:09:50 2023  
Response via : Initial Calibration

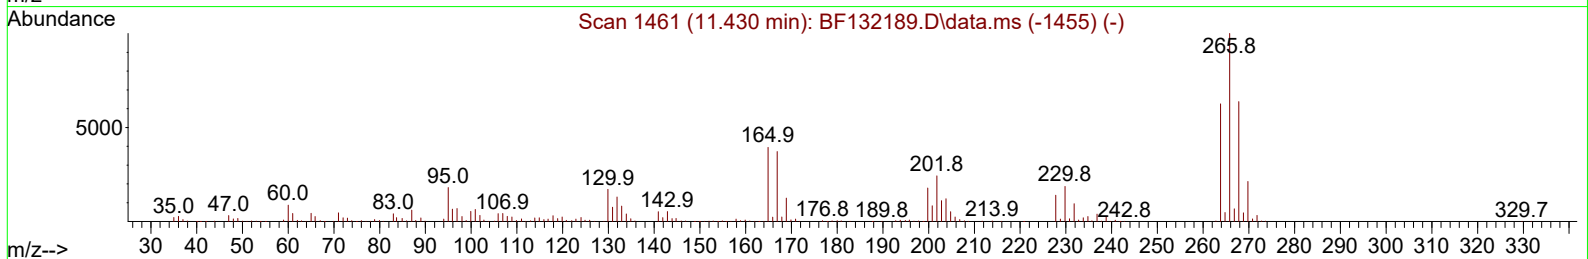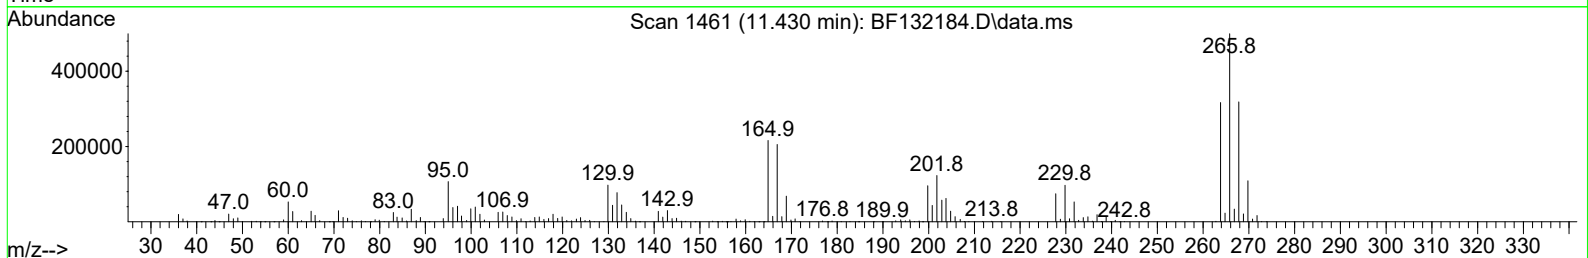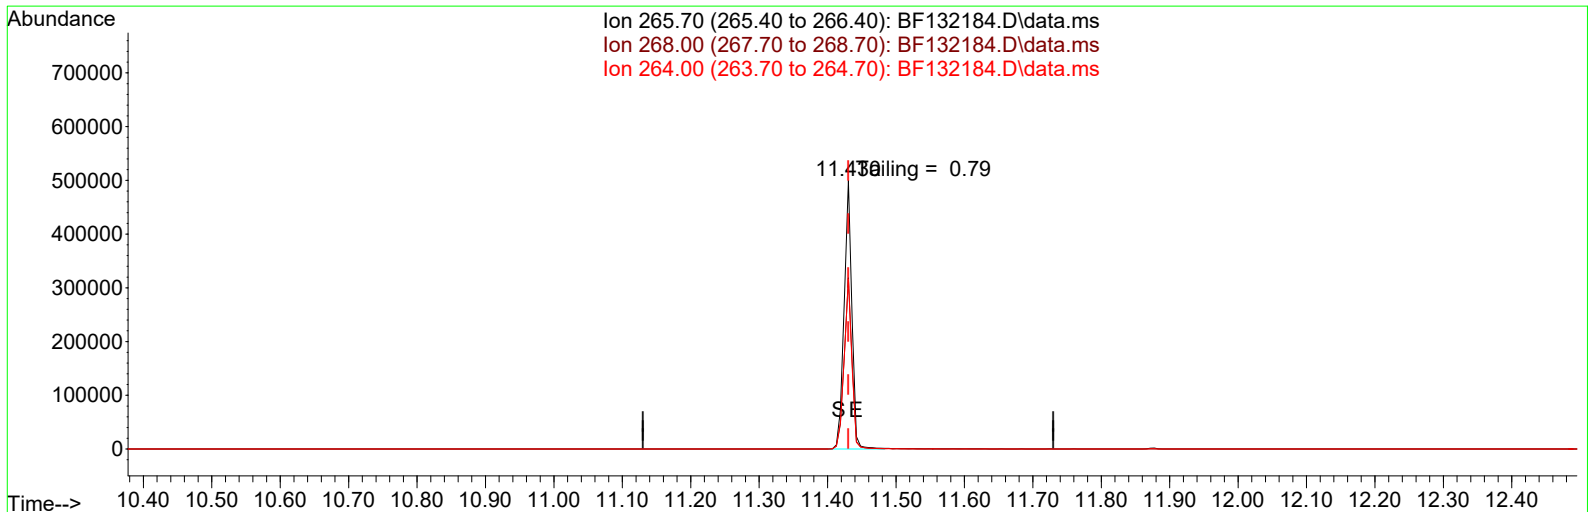

TIC: BF132184.D\data.ms

**(70) Pentachlorophenol (C)**

**11.430min (+ 0.000) 357864.42 ng**

**response 398862**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 63.73  |
| 264.00 | 62.60  | 63.40  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 1/24/2023     | BNA_F            | <u>BF132184.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 889780           | 13.813             |
| DDD           | 12511            | 13.536             |
| DDE           | 955              | 13.16              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 13466         | 903246           | 1.49               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP