

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012425\
 Data File : BF141257.D
 Acq On : 24 Jan 2025 12:43
 Operator : RC/JU
 Sample : PB166216BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166216BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	560	566	571	rBV	3182724	4398449	71.57%	12.576%
2	6.434	731	738	743	rBV	2985910	4386693	71.38%	12.542%
3	6.804	796	801	806	rBV	783161	966537	15.73%	2.763%
4	7.363	889	896	901	rBV	2171716	2948723	47.98%	8.431%
5	8.086	1013	1019	1024	rBV	961059	1295281	21.08%	3.703%
6	9.163	1195	1202	1208	rBV	4024228	5718894	93.05%	16.351%
7	9.839	1311	1317	1330	rBV	1074059	1488332	24.22%	4.255%
8	10.633	1445	1452	1469	rBV	2721728	3698410	60.18%	10.574%
9	11.333	1564	1571	1578	rBV	1155437	1486401	24.19%	4.250%
10	11.851	1654	1659	1672	rBV2	30062	70003	1.14%	0.200%
11	12.927	1835	1842	1847	rBV	4490000	6145869	100.00%	17.572%
12	13.986	2016	2022	2035	rBV	979532	1280377	20.83%	3.661%
13	15.480	2270	2276	2283	rBV	675299	1092131	17.77%	3.123%




Sum of corrected areas: 34976100

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012425\
Data File : BF141257.D
Acq On : 24 Jan 2025 12:43
Operator : RC/JU
Sample : PB166216BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166216BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

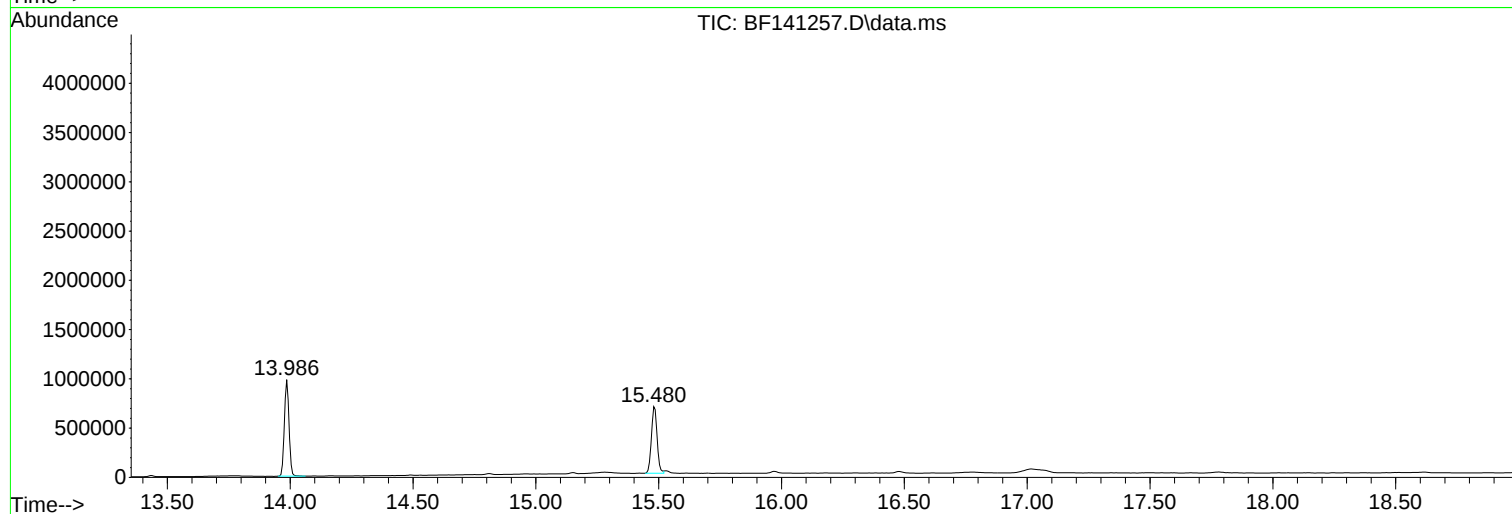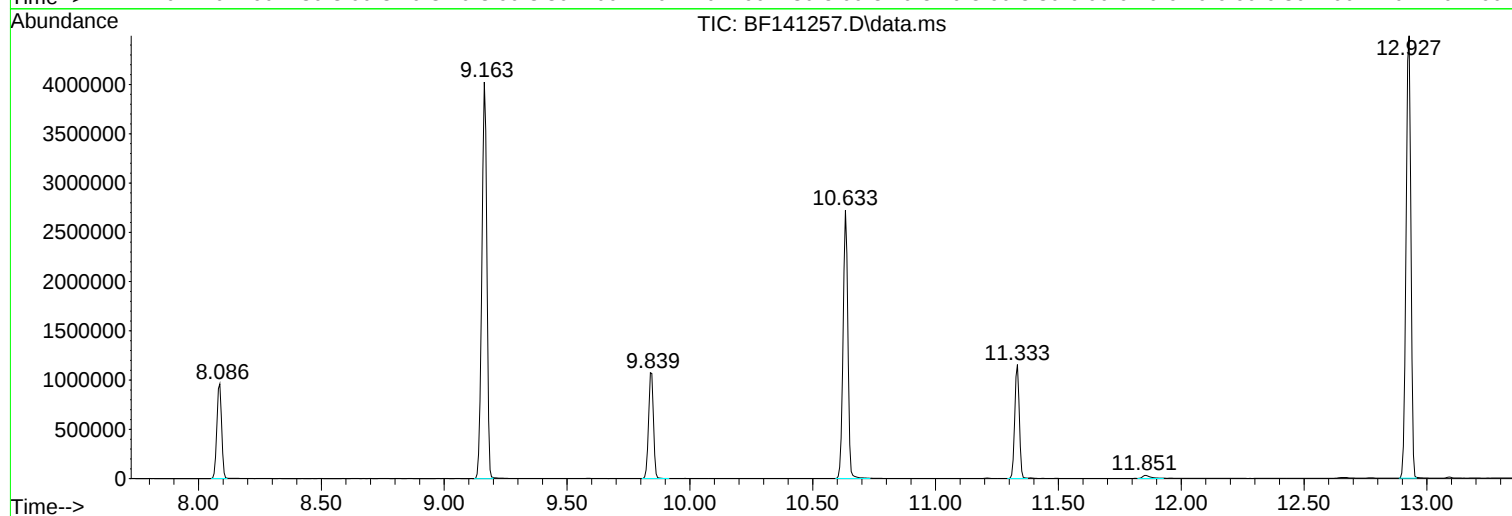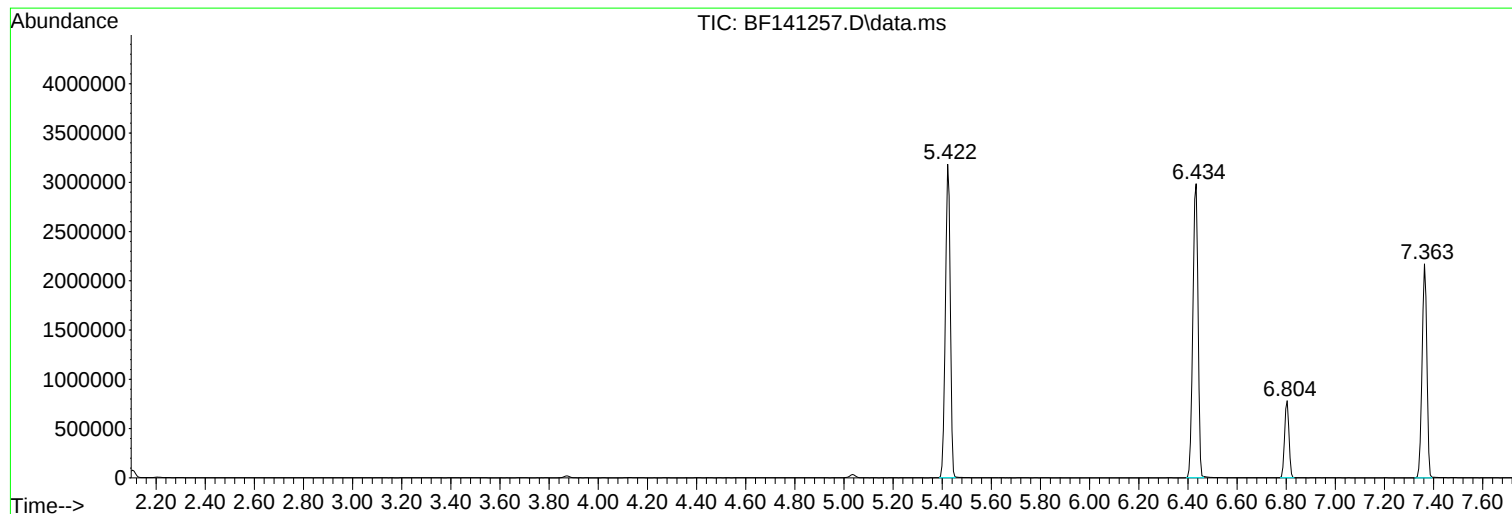

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012425\
Data File : BF141257.D
Acq On : 24 Jan 2025 12:43
Operator : RC/JU
Sample : PB166216BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166216BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012425\
Data File : BF141257.D
Acq On : 24 Jan 2025 12:43
Operator : RC/JU
Sample : PB166216BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166216BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------