


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012425\
Data File : BF141255.D
Acq On : 24 Jan 2025 10:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 10 22:54:19 2025

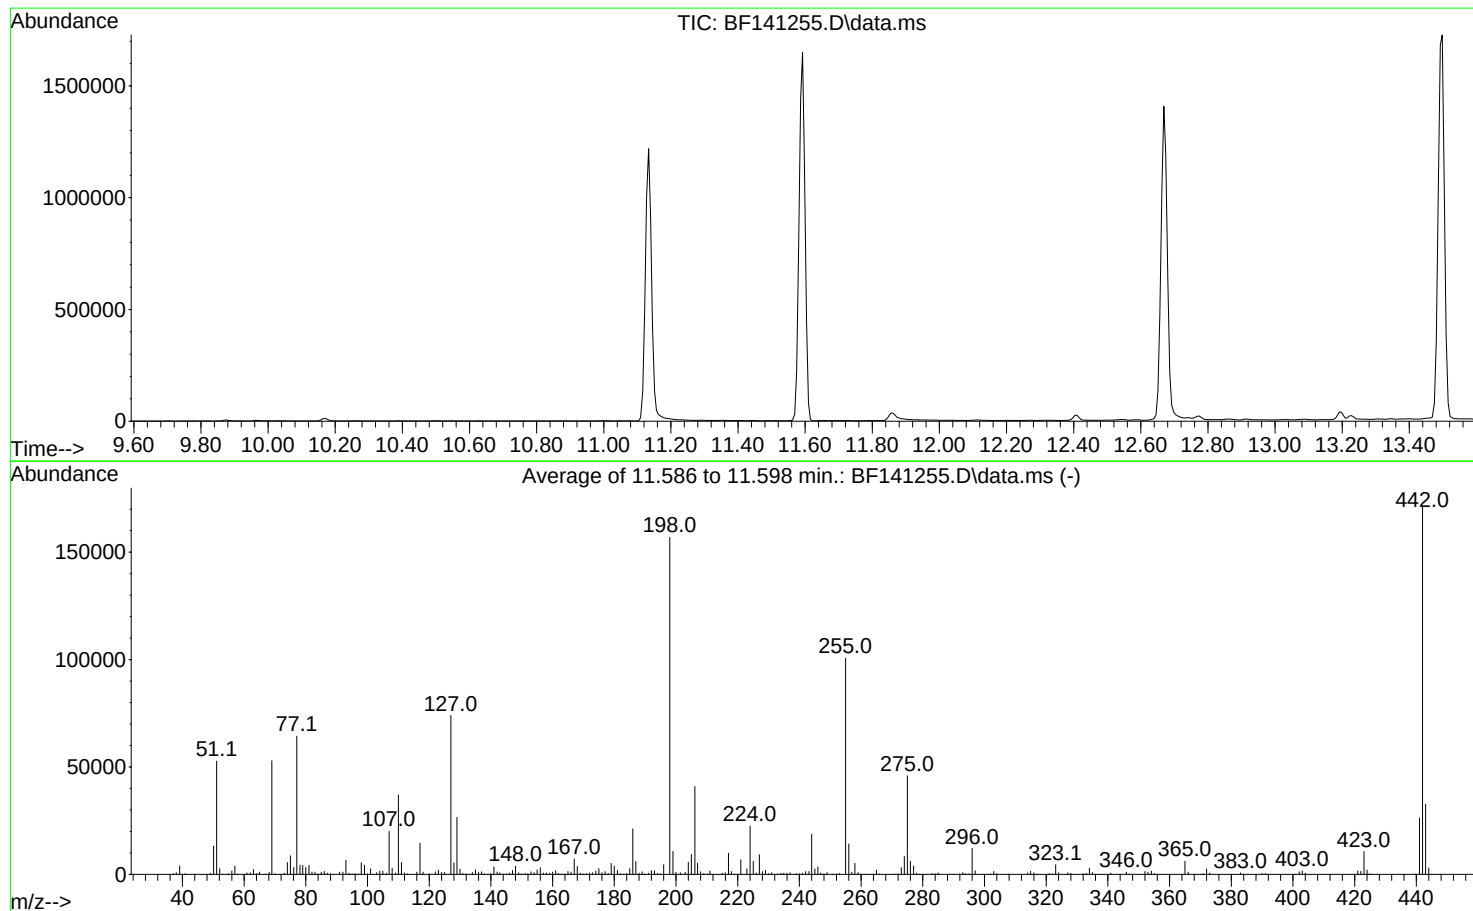

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	52672	PASS
68	69	0.00	2	1.9	1012	PASS
69	198	0.00	100	33.7	52877	PASS
70	69	0.00	2	0.6	324	PASS
127	198	10	80	47.1	73971	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	156888	PASS
199	198	5	9	6.8	10676	PASS
275	198	10	60	29.2	45877	PASS
365	198	1	100	3.9	6089	PASS
441	198	0.01	100	16.7	26208	PASS
442	442	50	100	100.0	171264	PASS
443	442	15	24	19.1	32733	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/24/2025	BNA_F	<u>BF141255.D</u>
Compound Name	Response	Retention Time
DDT	455229	13.498
DDD	13353	13.192
DDE	1195	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14548	469777	3.10

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012425\
Data File : BF141255.D
Acq On : 24 Jan 2025 10:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 25 00:53:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

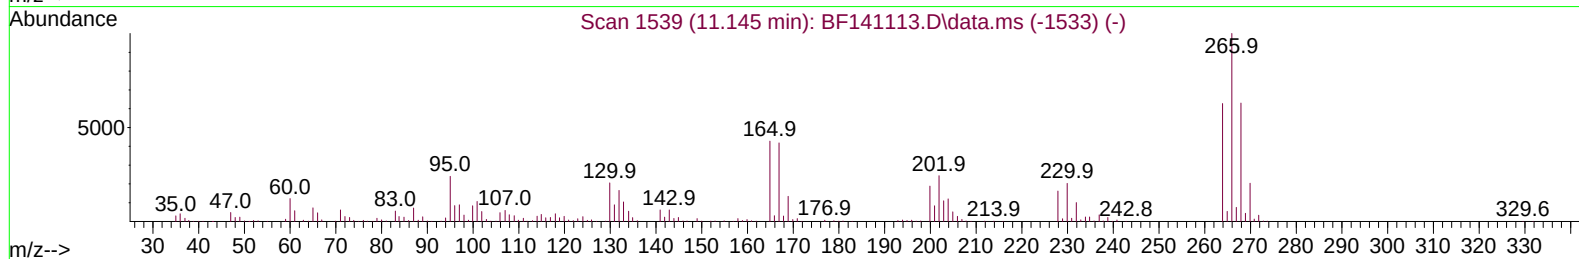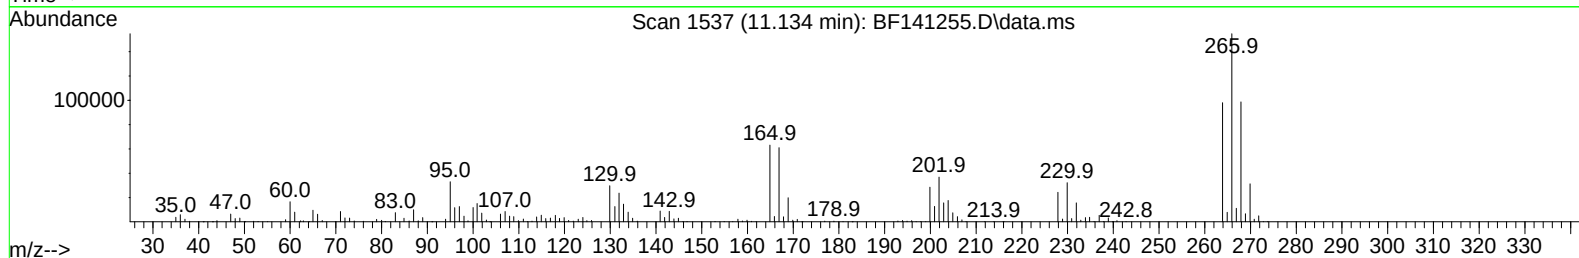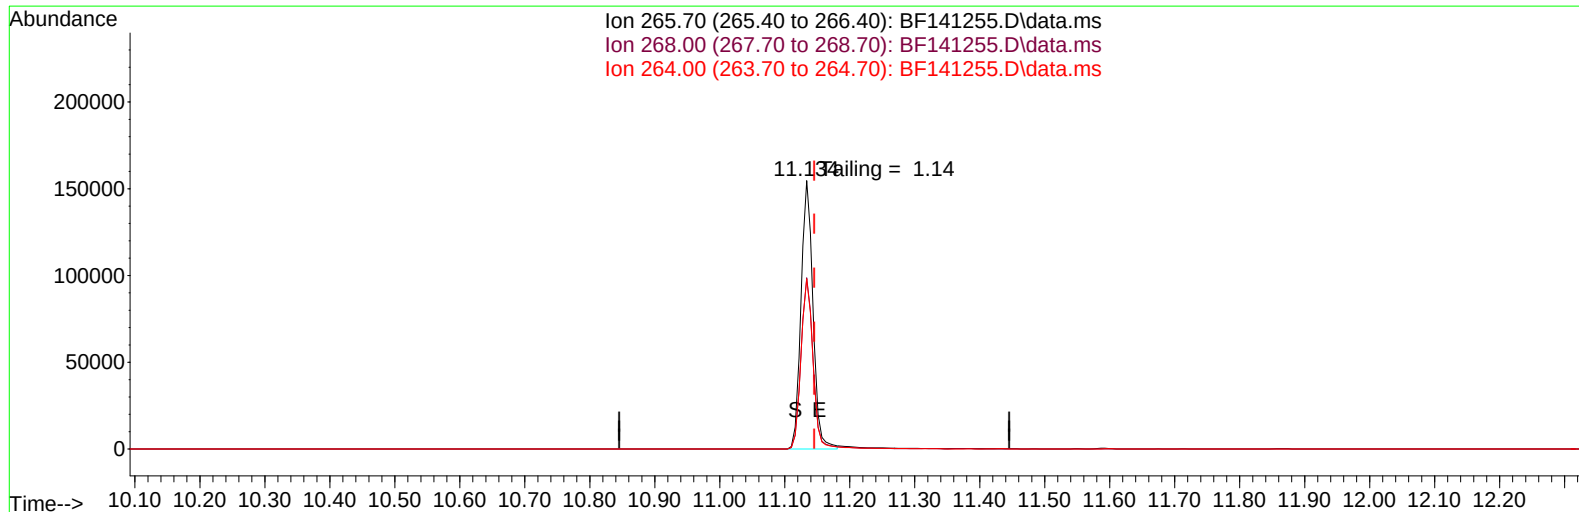

TIC: BF141255.D\data.ms

(70) Pentachlorophenol (C)

11.134min (-0.012) 29479.71 ng


response 204451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.79
264.00	62.70	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012425\
Data File : BF141255.D
Acq On : 24 Jan 2025 10:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 25 00:53:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 22:54:19 2025
Response via : Initial Calibration

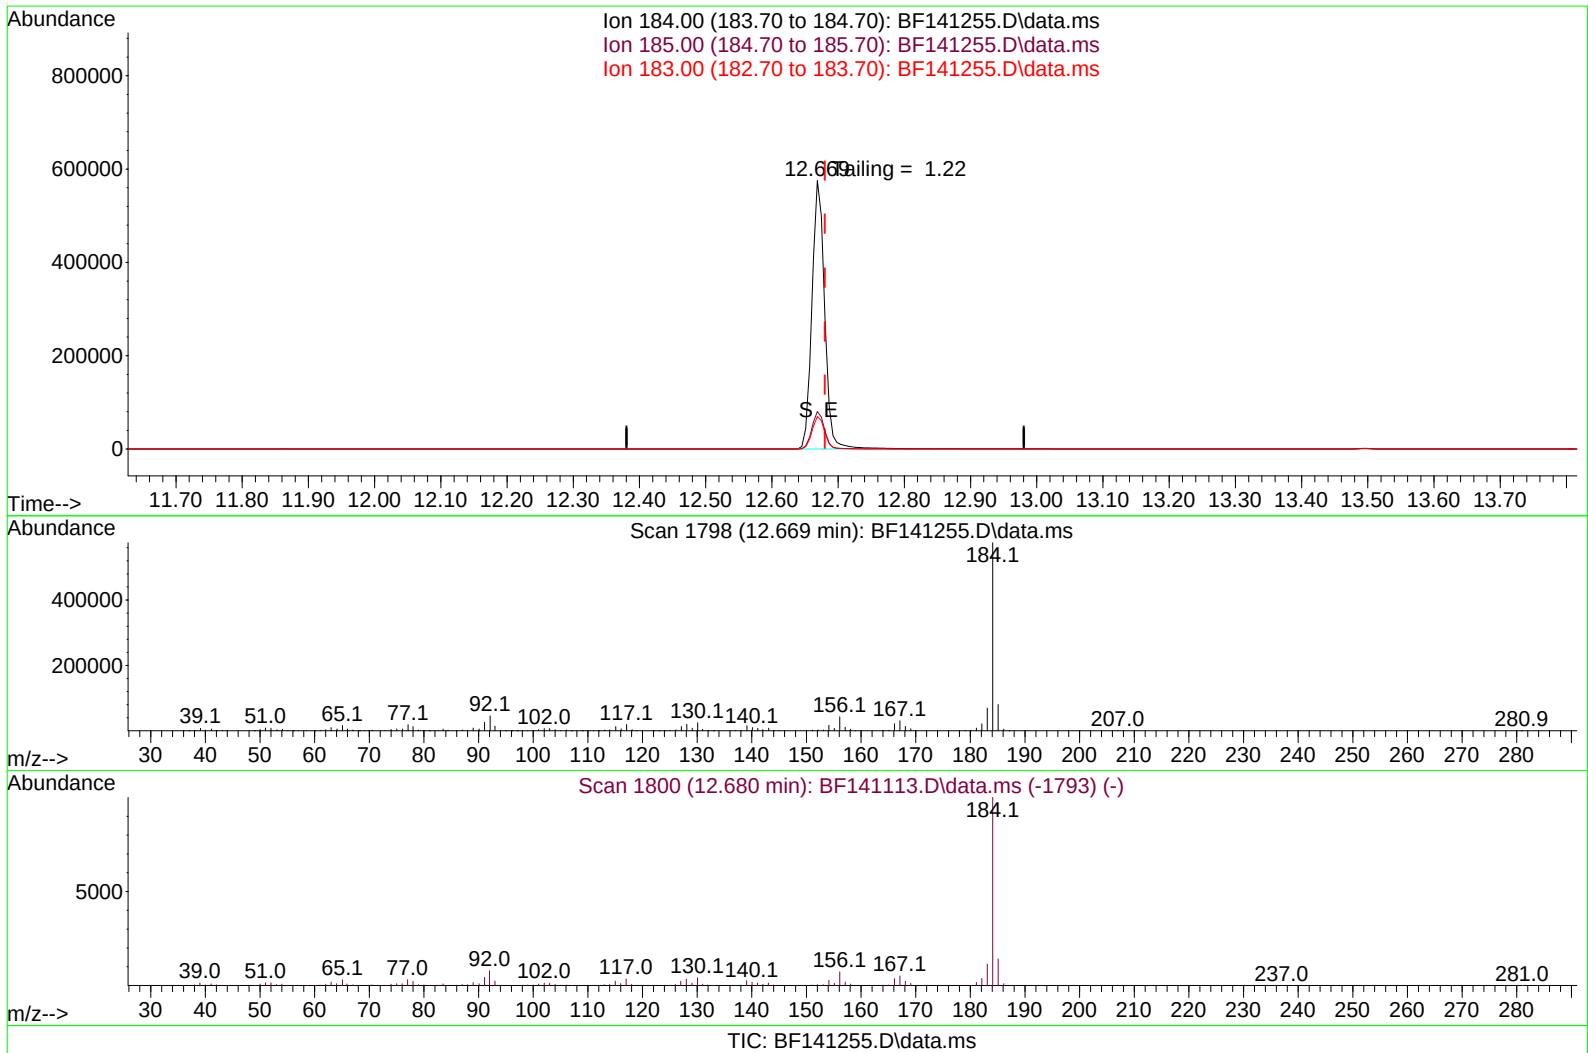

(77) Benzidine

12.669min (-0.012) 62741.67 ng

response 766750

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.96
183.00	11.50	12.09
0.00	0.00	0.00