

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012516\
 Data File : BF084610.D
 Acq On : 25 Jan 2016 16:36
 Operator : SJ/IZ
 Sample : H1201-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-03

Quant Time: Jan 25 17:05:33 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 25 16:24:07 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	200036	20.00	ng	0.00
21) Naphthalene-d8	8.02	136	800344	20.00	ng	-0.01
38) Acenaphthene-d10	9.77	164	417921	20.00	ng	-0.01
63) Phenanthrene-d10	11.25	188	829546	20.00	ng	-0.01
75) Chrysene-d12	13.88	240	720522	20.00	ng	-0.01
86) Perylene-d12	15.28	264	557287	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	942320	76.19	ng	0.00
7) Phenol-d6	6.38	99	895387	57.65	ng	-0.01
23) Nitrobenzene-d5	7.31	82	1654710	115.07	ng	0.00
41) 2,4,6-Tribromophenol	10.57	330	695339	164.80	ng	0.00
44) 2-Fluorobiphenyl	9.10	172	2381730	101.48	ng	0.00
78) Terphenyl-d14	12.84	244	2581698	79.98	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012516\
Data File : BF084610.D
Acq On : 25 Jan 2016 16:36
Operator : SJ/IZ
Sample : H1201-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-03

Quant Time: Jan 25 17:05:33 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 25 16:24:07 2016
Response via : Initial Calibration

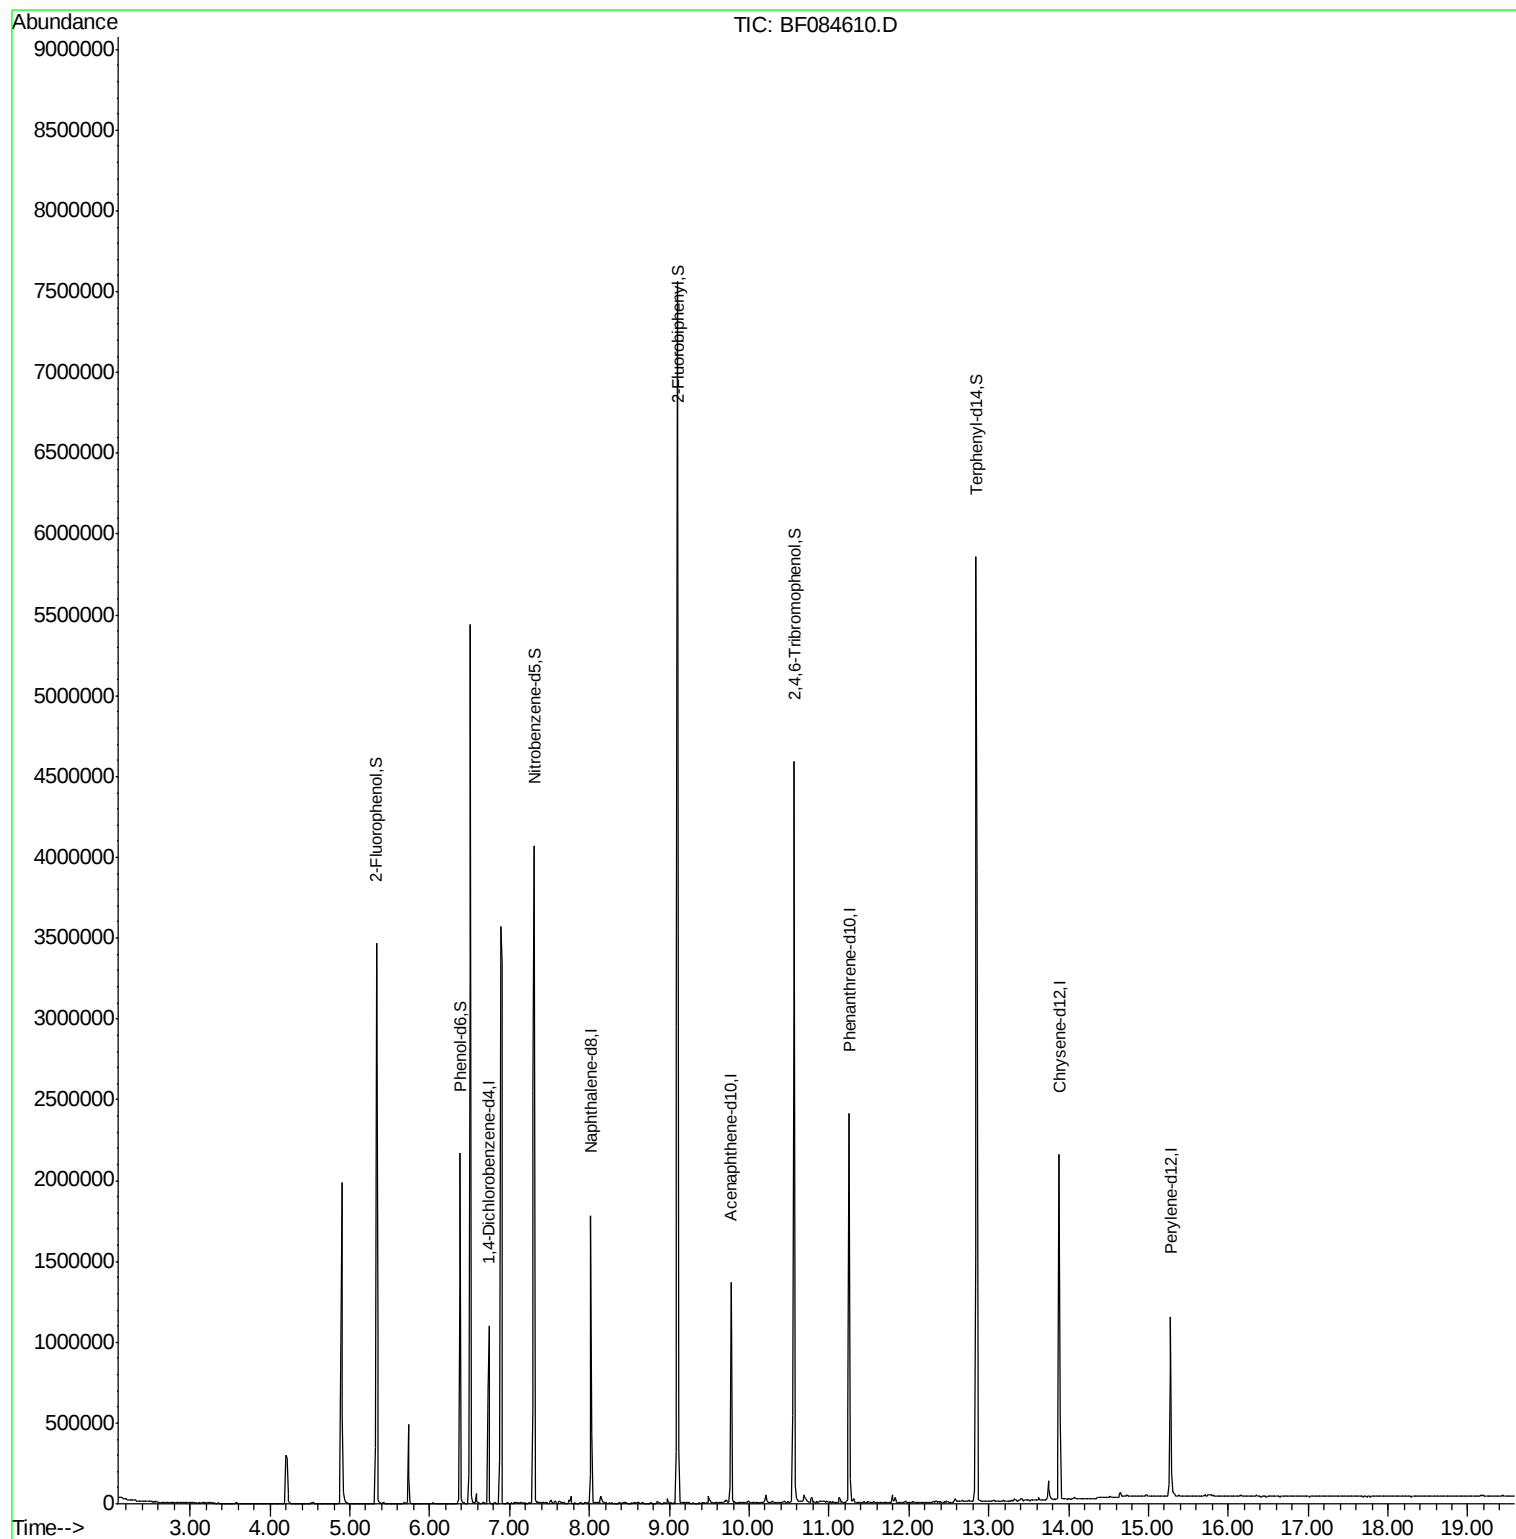

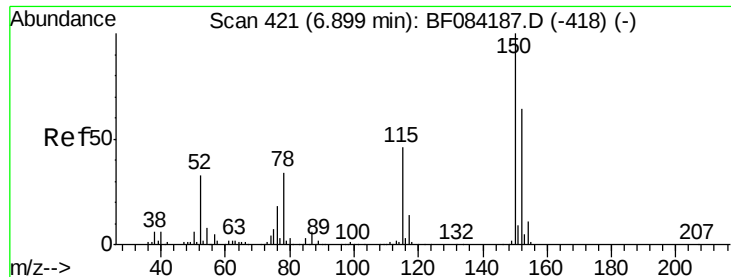

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.74 min Scan# 407

Delta R.T. 0.00 min

Lab File: BF084610.D

Acq: 25 Jan 2016 16:36

Instrument :

BNA_F

ClientSampleId :

MW-03


Tot Ion:152 Resp: 200036

Ion Ratio Lower Upper

152 100

150 156.5 123.0 184.4




115 60.1 51.4 77.2

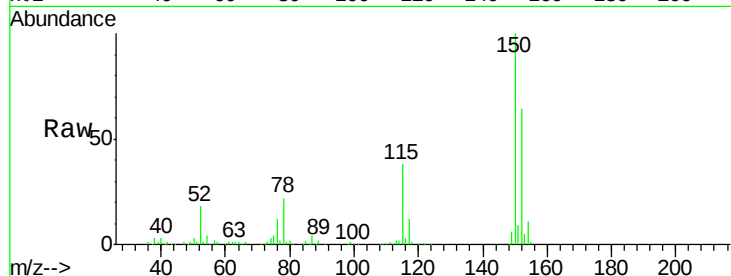

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

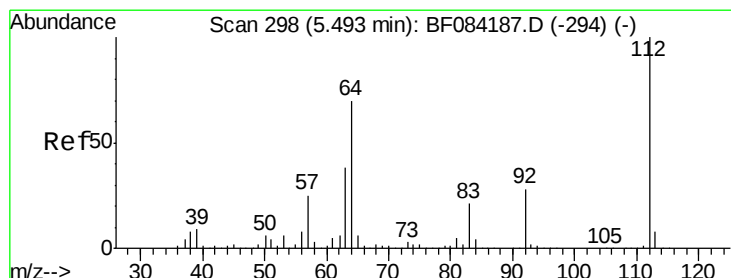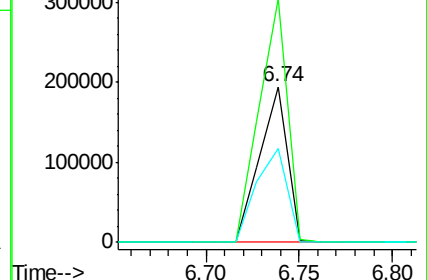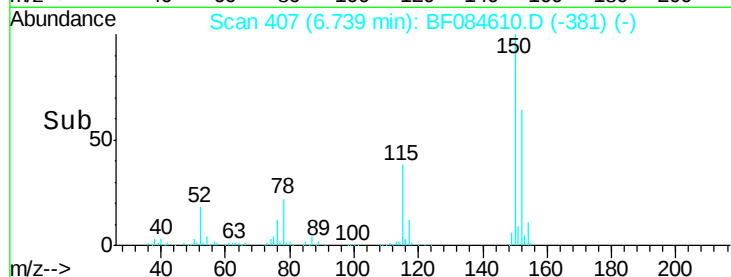

#5

2-Fluorophenol

Concen: 76.19 ng

RT: 5.33 min Scan# 284

Delta R.T. 0.00 min

Lab File: BF084610.D

Acq: 25 Jan 2016 16:36


Tgt Ion:112 Resp: 942320

Ion Ratio Lower Upper

112 100

64 66.7 36.6 55.0#



63 35.8 19.4 29.0#

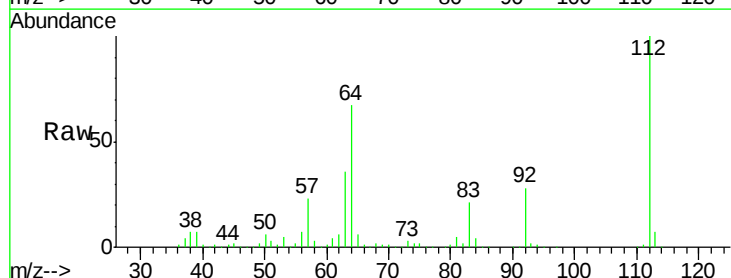


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

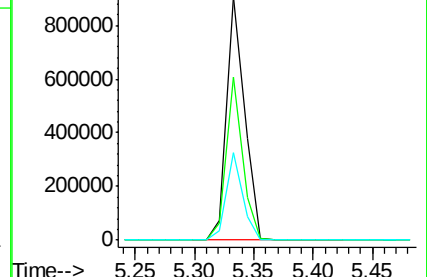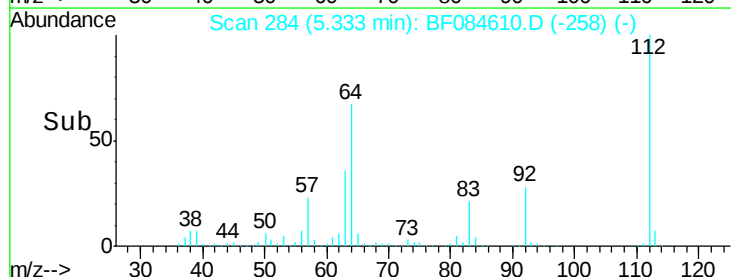

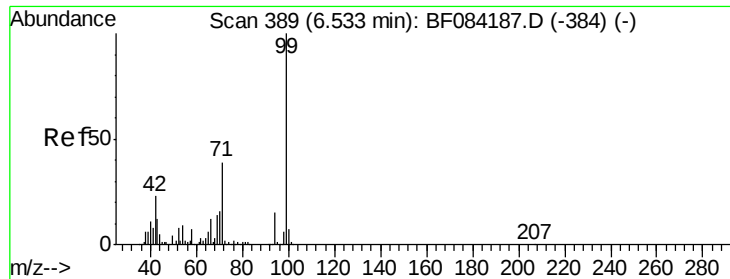

#7

Phenol-d6

Concen: 57.65 ng

RT: 6.38 min Scan# 376

Delta R.T. -0.01 min

Lab File: BF084610.D

Acq: 25 Jan 2016 16:36

Instrument :

BNA_F

ClientSampled :

MW-03


Tot Ion: 99 Resp: 895387

Ion Ratio Lower Upper

99 100

42 15.8 12.8 19.2




71 31.8 30.9 46.3

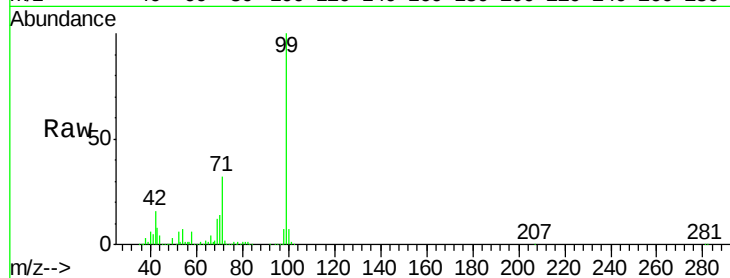

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

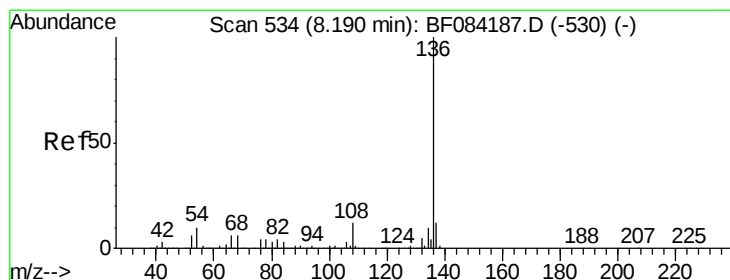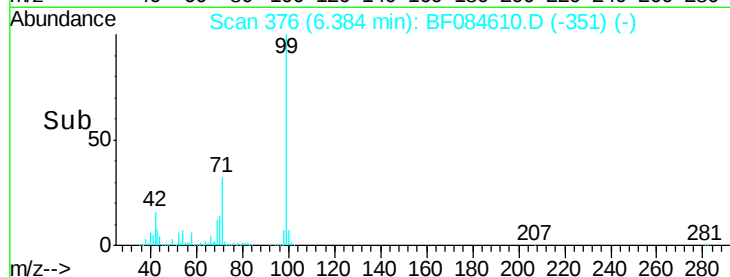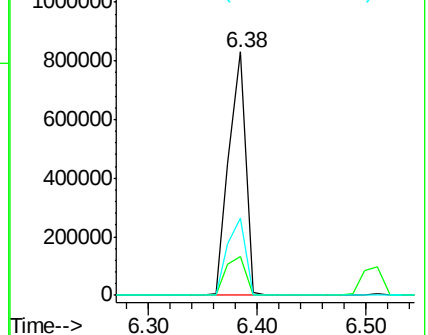

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.02 min Scan# 519

Delta R.T. -0.01 min

Lab File: BF084610.D

Acq: 25 Jan 2016 16:36

Tgt Ion: 136 Resp: 800344


Ion Ratio Lower Upper

136 100

137 11.5 8.7 13.1

54 9.8 5.8 8.8#

68 5.3 4.2 6.2


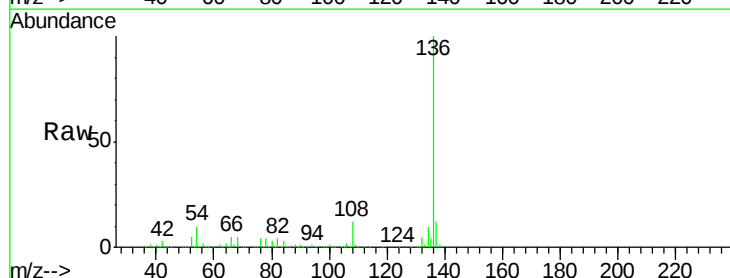



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

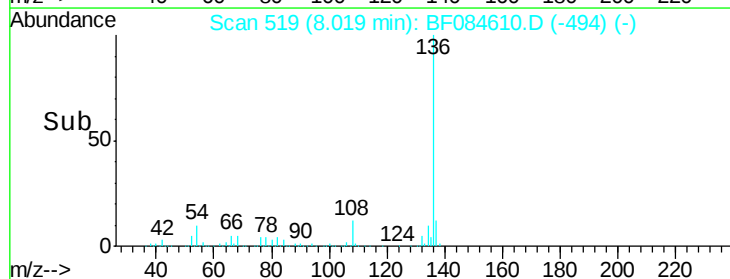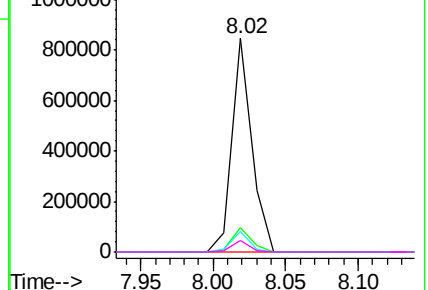




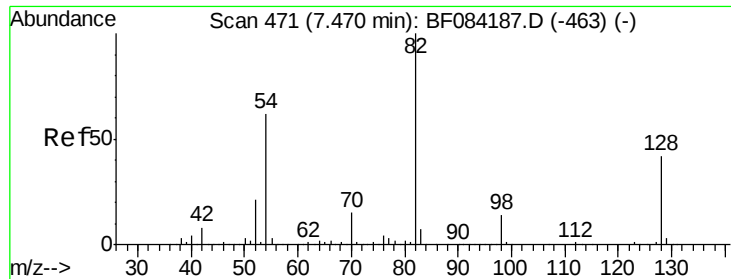


#23
 Nitrobenzene-d5
 Concen: 115.07 ng
 RT: 7.31 min Scan# 457
 Delta R.T. 0.00 min
 Lab File: BF084610.D
 Acq: 25 Jan 2016 16:36

Instrument :
 BNA_F
 ClientSampled :
 MW-03

Tot Ion: 82 Resp: 1654710




Ion	Ratio	Lower	Upper
82	100		
128	47.4	34.6	51.8
54	54.8	38.4	57.6

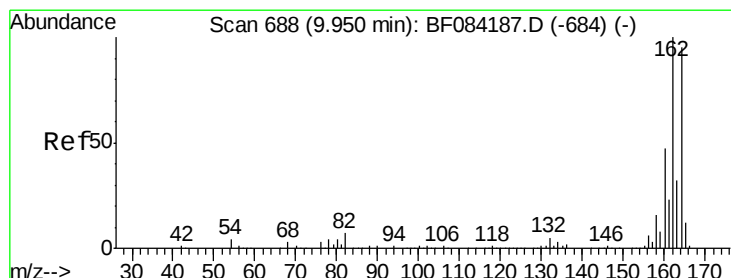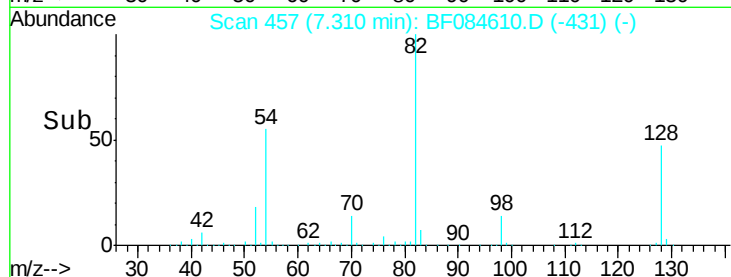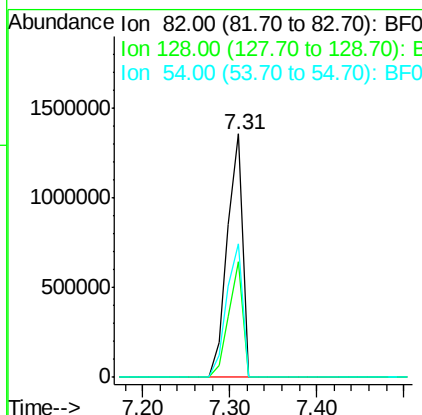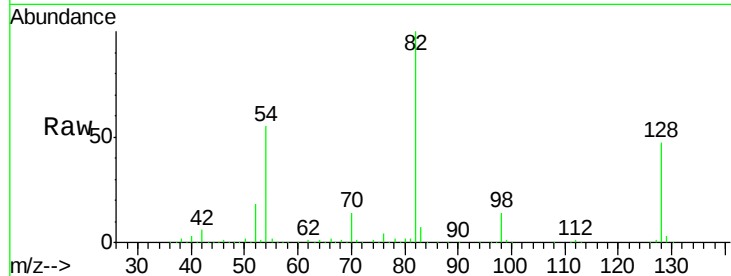


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.77 min Scan# 672
 Delta R.T. -0.01 min
 Lab File: BF084610.D
 Acq: 25 Jan 2016 16:36

Tgt Ion:164 Resp: 417921

Ion	Ratio	Lower	Upper
164	100		
162	103.2	85.1	127.7
160	46.0	37.5	56.3

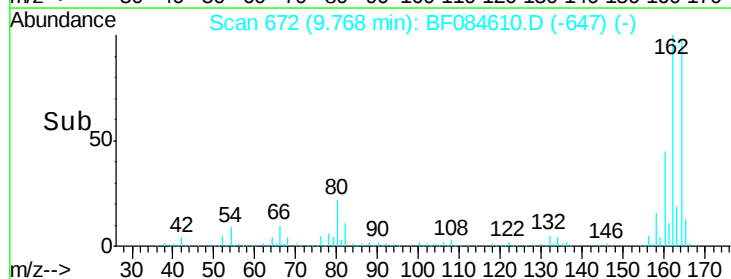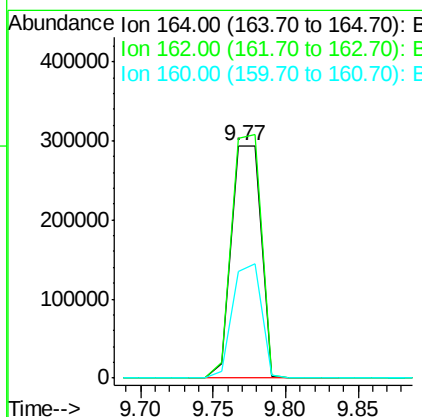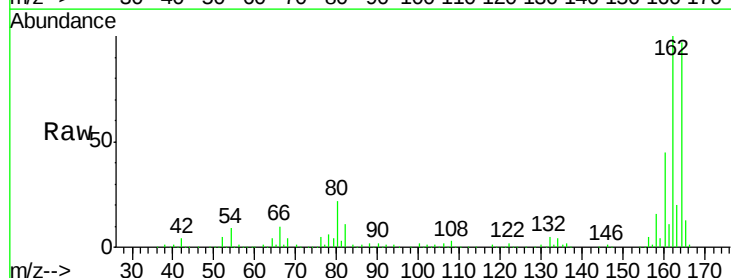

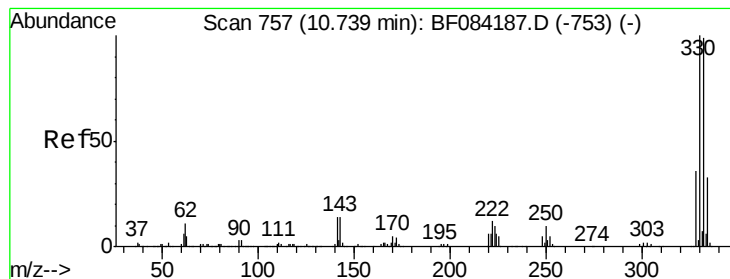

#41

2,4,6-Tribromophenol

Concen: 164.80 ng

RT: 10.57 min Scan# 742

Delta R.T. 0.00 min

Lab File: BF084610.D

Acq: 25 Jan 2016 16:36

Instrument :

BNA_F

ClientSampleId :

MW-03


Tot Ion:330 Resp: 695339

Ion Ratio Lower Upper




330 100

332 96.7 76.6 114.8

141 38.8 27.8 41.6

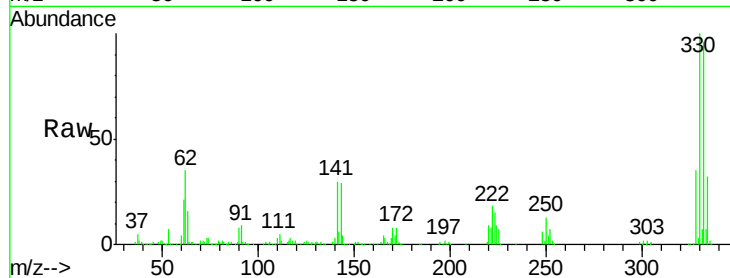

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

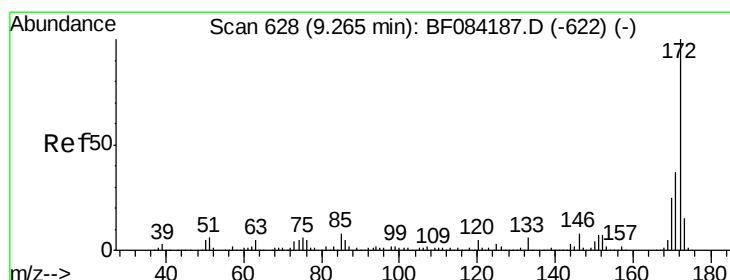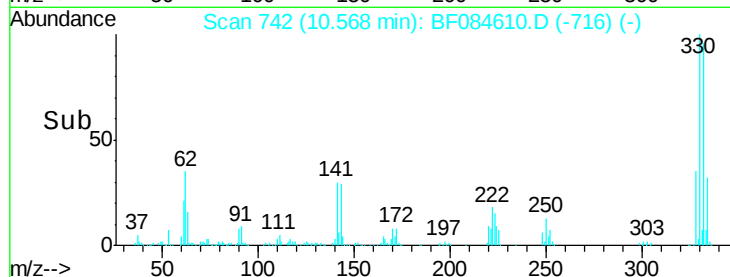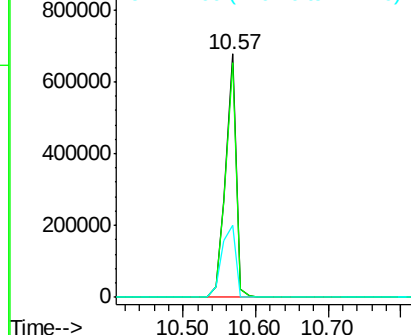

#44

2-Fluorobiphenyl

Concen: 101.48 ng

RT: 9.10 min Scan# 614

Delta R.T. 0.00 min

Lab File: BF084610.D

Acq: 25 Jan 2016 16:36


Tgt Ion:172 Resp: 2381730

Ion Ratio Lower Upper



172 100


171 38.0 28.9 43.3

170 26.4 18.6 27.8

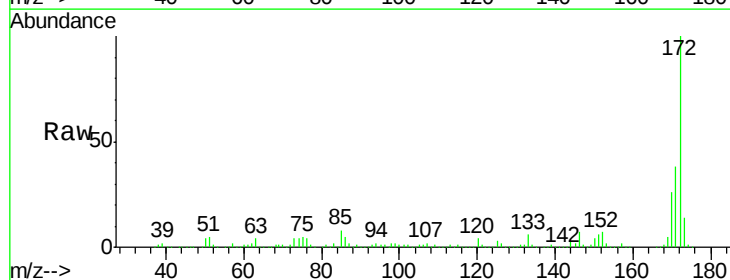

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

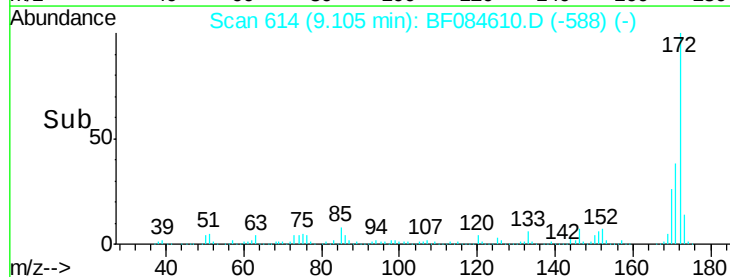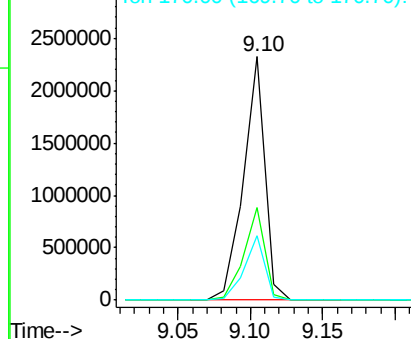

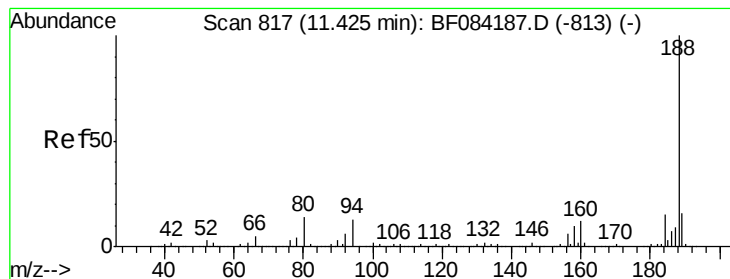

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.25 min Scan# 802

Delta R.T. -0.01 min

Lab File: BF084610.D

Acq: 25 Jan 2016 16:36

Instrument :

BNA_F

ClientSampleId :

MW-03


Tot Ion:188 Resp: 829546

Ion Ratio Lower Upper

188 100

94 8.5 9.0 13.4#




80 9.2 9.6 14.4#

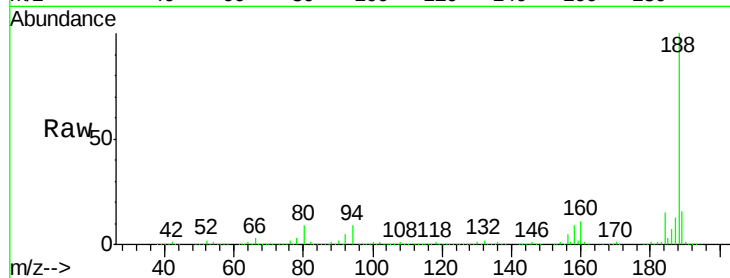

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

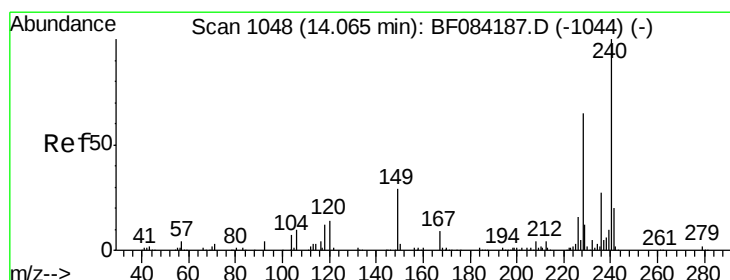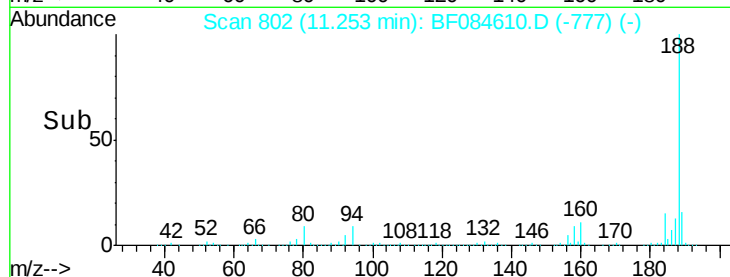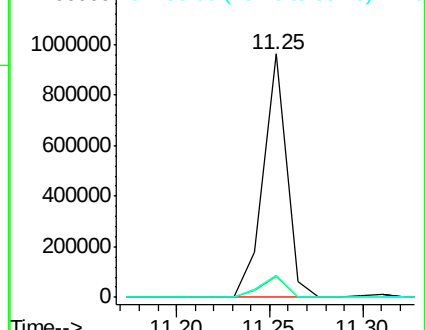

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.88 min Scan# 1032

Delta R.T. -0.01 min

Lab File: BF084610.D

Acq: 25 Jan 2016 16:36


Tgt Ion:240 Resp: 720522

Ion Ratio Lower Upper

240 100

120 12.9 9.5 14.3



236 26.5 20.6 31.0

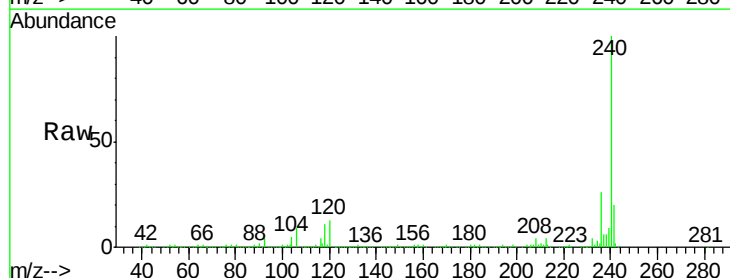


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

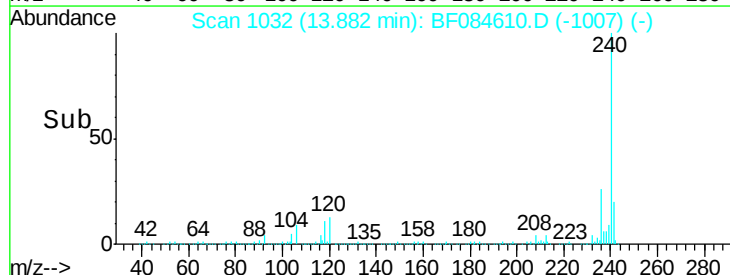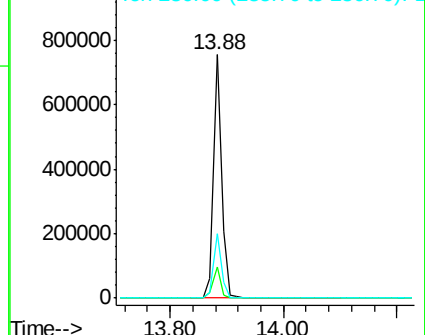


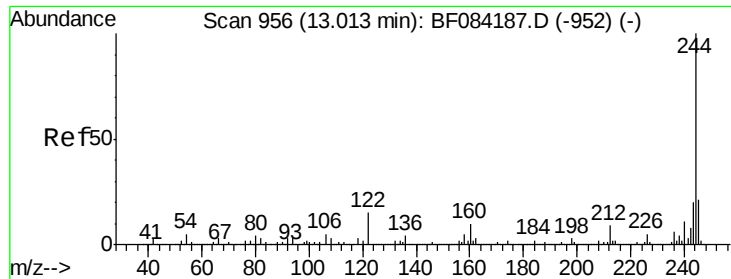




#78
 Terphenyl-d14
 Concen: 79.98 ng
 RT: 12.84 min Scan# 941
 Delta R.T. -0.01 min
 Lab File: BF084610.D
 Acq: 25 Jan 2016 16:36

Instrument :
 BNA_F
 ClientSampleId :
 MW-03

Tot Ion:244 Resp: 2581698
 Ion Ratio Lower Upper
 244 100
 212 8.1 5.7 8.5
 122 15.6 7.4 11.0#

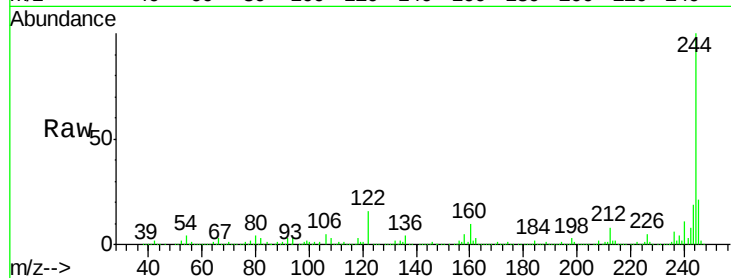


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

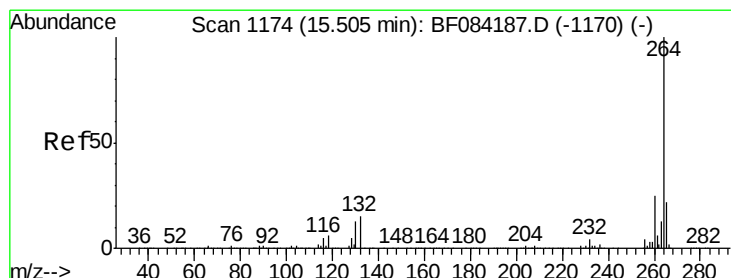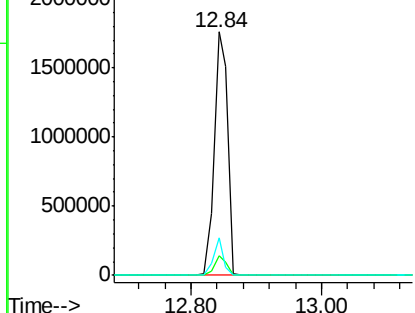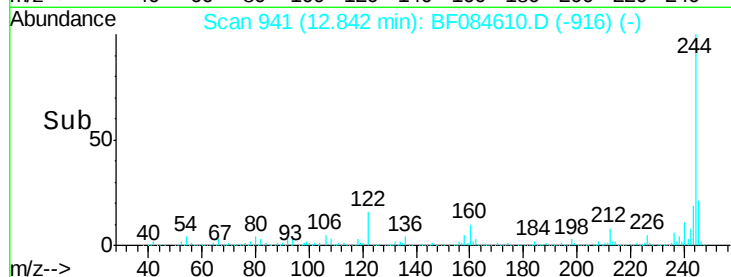

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.28 min Scan# 1154
 Delta R.T. 0.00 min
 Lab File: BF084610.D
 Acq: 25 Jan 2016 16:36

Tgt Ion:264 Resp: 557287
 Ion Ratio Lower Upper
 264 100
 260 23.6 19.4 29.2
 265 22.0 17.8 26.6

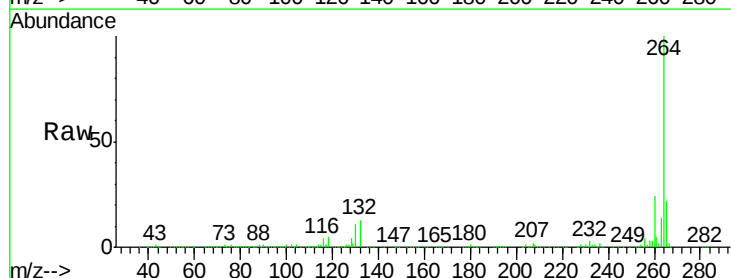

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

