


Data Path : Z:\HPCHEM1\BNA F\DATA\BF012516\
 Data File : BF084601.D
 Acq On : 25 Jan 2016 11:34
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 25 16:24:07 2016

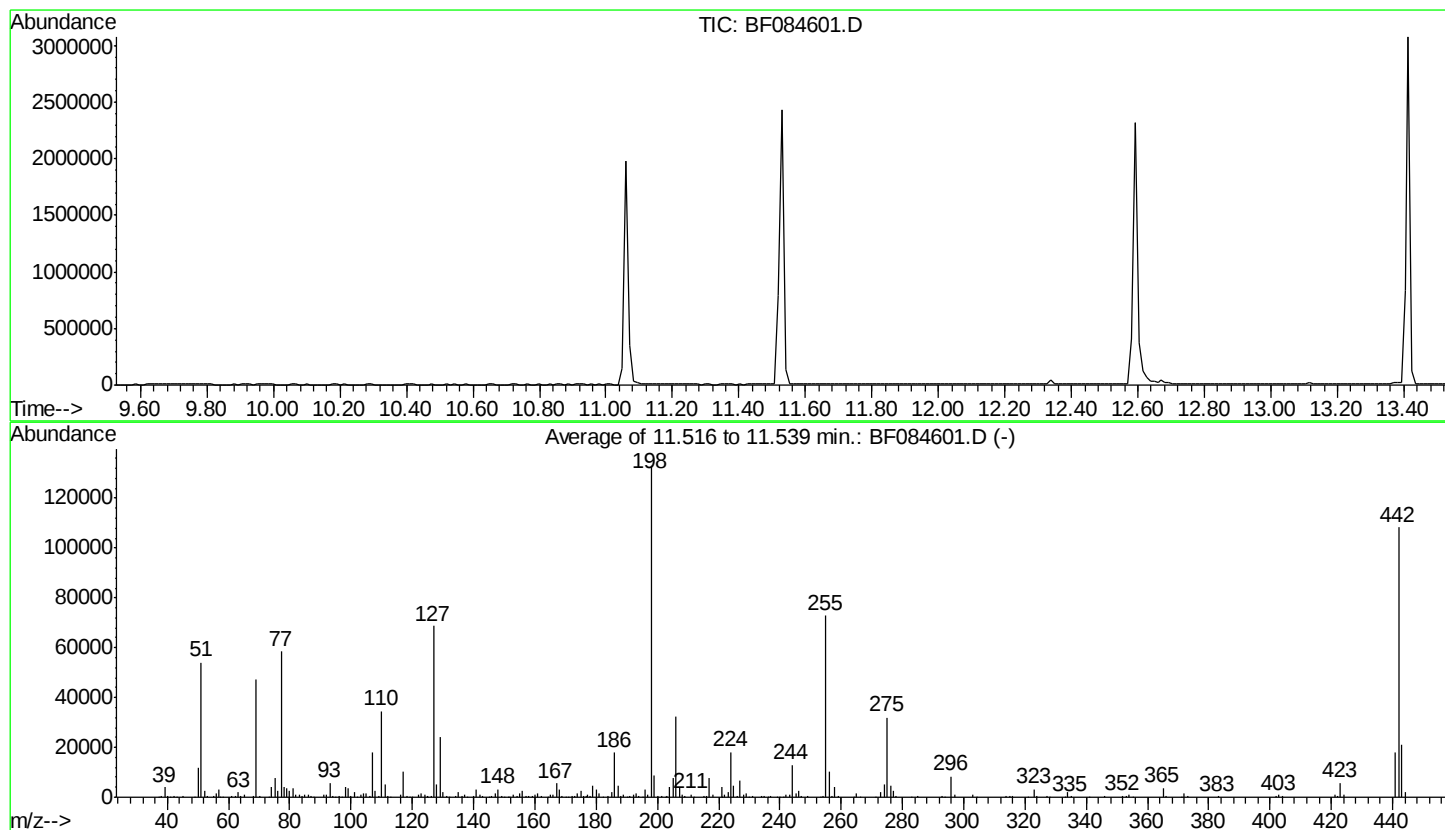

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	53998	PASS
68	69	0.00	2	1.5	717	PASS
69	198	0.00	100	35.6	47314	PASS
70	69	0.00	2	0.9	425	PASS
127	198	10	80	51.7	68797	PASS
197	198	0.00	2	0.6	845	PASS
198	198	100	100	100.0	133085	PASS
199	198	5	9	6.7	8933	PASS
275	198	10	60	24.1	32026	PASS
365	198	1	100	2.9	3794	PASS
441	442	0.01	24	16.5	17807	PASS
442	198	50	100	81.3	108221	PASS
443	442	15	24	19.4	20991	PASS