
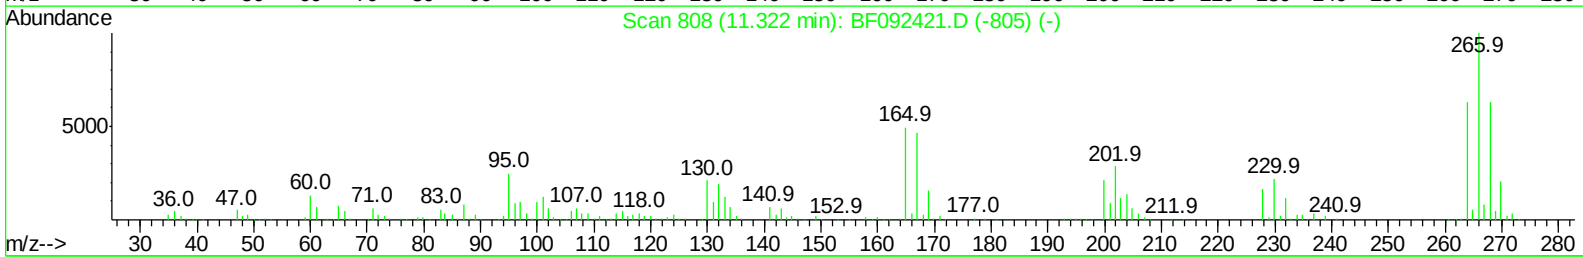
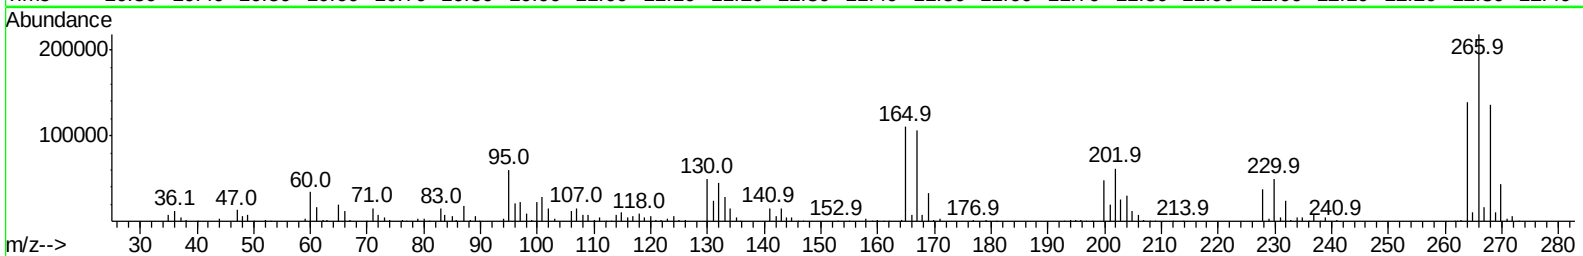


Data Path : Z:\HPCHEM1\BNA F\DATA\BF012517\
Data File : BF092463.D
Acq On : 25 Jan 2017 9:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 13:08:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

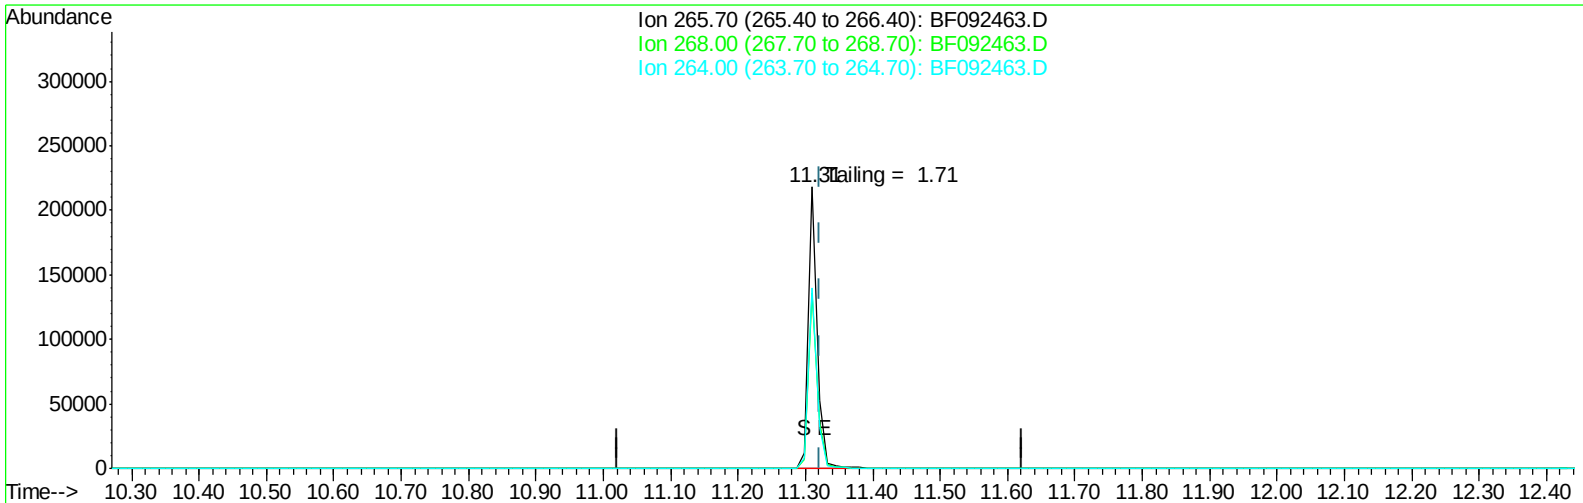

TIC: BF092463.D

(69) Pentachlorophenol (C)




11.311min (-0.012) 49747.42ng

response 200610

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.49
264.00	62.90	64.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012517\
Data File : BF092463.D
Acq On : 25 Jan 2017 9:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 13:08:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

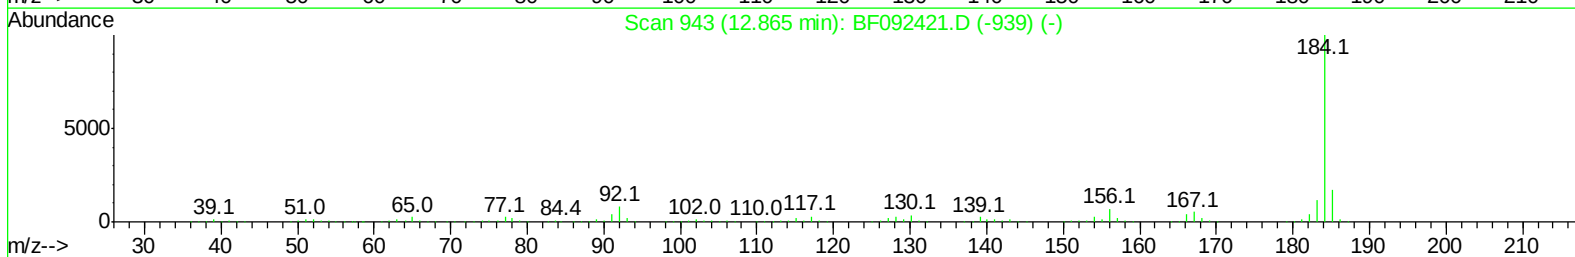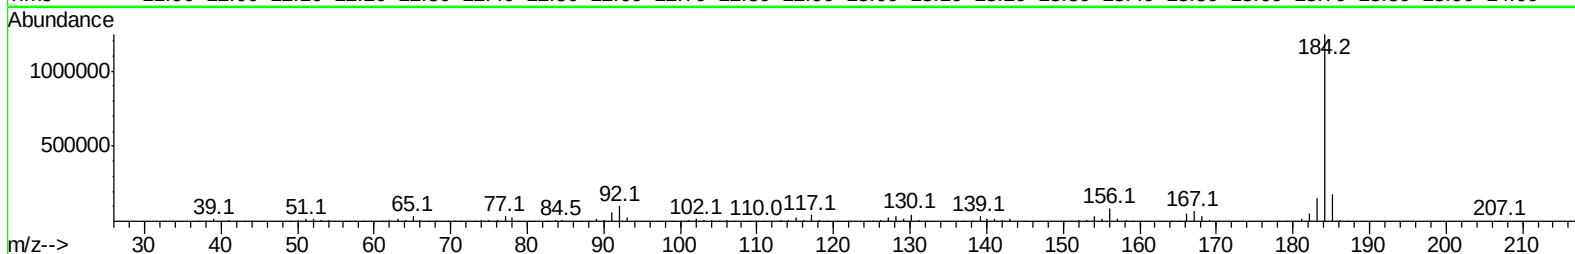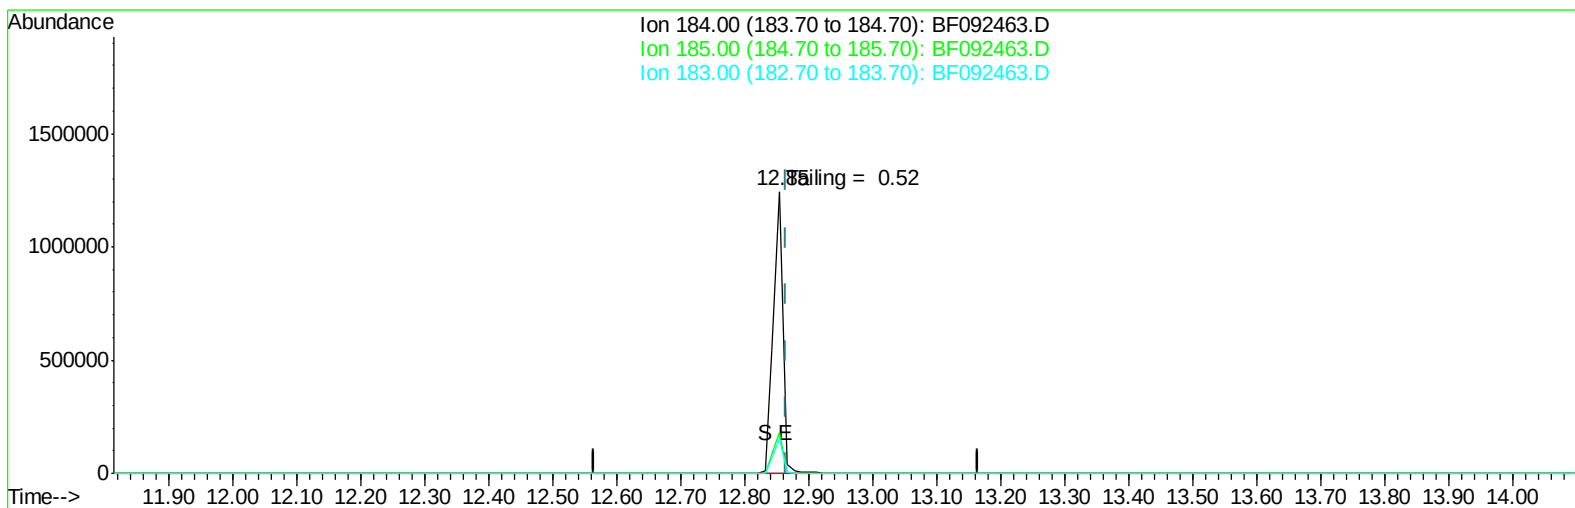

TIC: BF092463.D

(76) Benzidine

12.854min (-0.012) 0.00ng

response 1287387

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.58
183.00	11.50	12.51
0.00	0.00	0.00