

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012517\
 Data File : BF092476.D
 Acq On : 25 Jan 2017 15:05
 Operator : SJ/MA
 Sample : PB96241BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB96241BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.173	266	270	279	rVB	1245694	2115726	37.86%	4.631%
2	5.573	302	305	307	rBV	4289630	4999622	89.47%	10.944%
3	6.590	390	394	396	rBV	4169501	4758450	85.15%	10.416%
4	6.727	403	406	409	rBV	3363202	4838654	86.59%	10.591%
5	6.967	424	427	429	rBV	1276192	1140013	20.40%	2.495%
6	7.127	438	441	443	rBV	3340051	3798755	67.98%	8.315%
7	7.527	473	476	479	rBV	2411948	3066435	54.88%	6.712%
8	8.259	537	540	542	rBV	1508231	1558477	27.89%	3.411%
9	9.345	631	635	637	rBV	4633260	5587998	100.00%	12.232%
10	10.019	691	694	697	rBV	1641024	1669088	29.87%	3.654%
11	10.808	760	763	766	rBV2	2236139	2914597	52.16%	6.380%
12	11.505	822	824	827	rVB2	1394175	1657589	29.66%	3.628%
13	13.105	961	964	966	rBV	4500659	4857245	86.92%	10.632%
14	14.145	1053	1055	1058	rBV	1243953	1520286	27.21%	3.328%
15	15.631	1181	1185	1188	rBV	820659	1201545	21.50%	2.630%


Sum of corrected areas: 45684480

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012517\
Data File : BF092476.D
Acq On : 25 Jan 2017 15:05
Operator : SJ/MA
Sample : PB96241BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96241BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

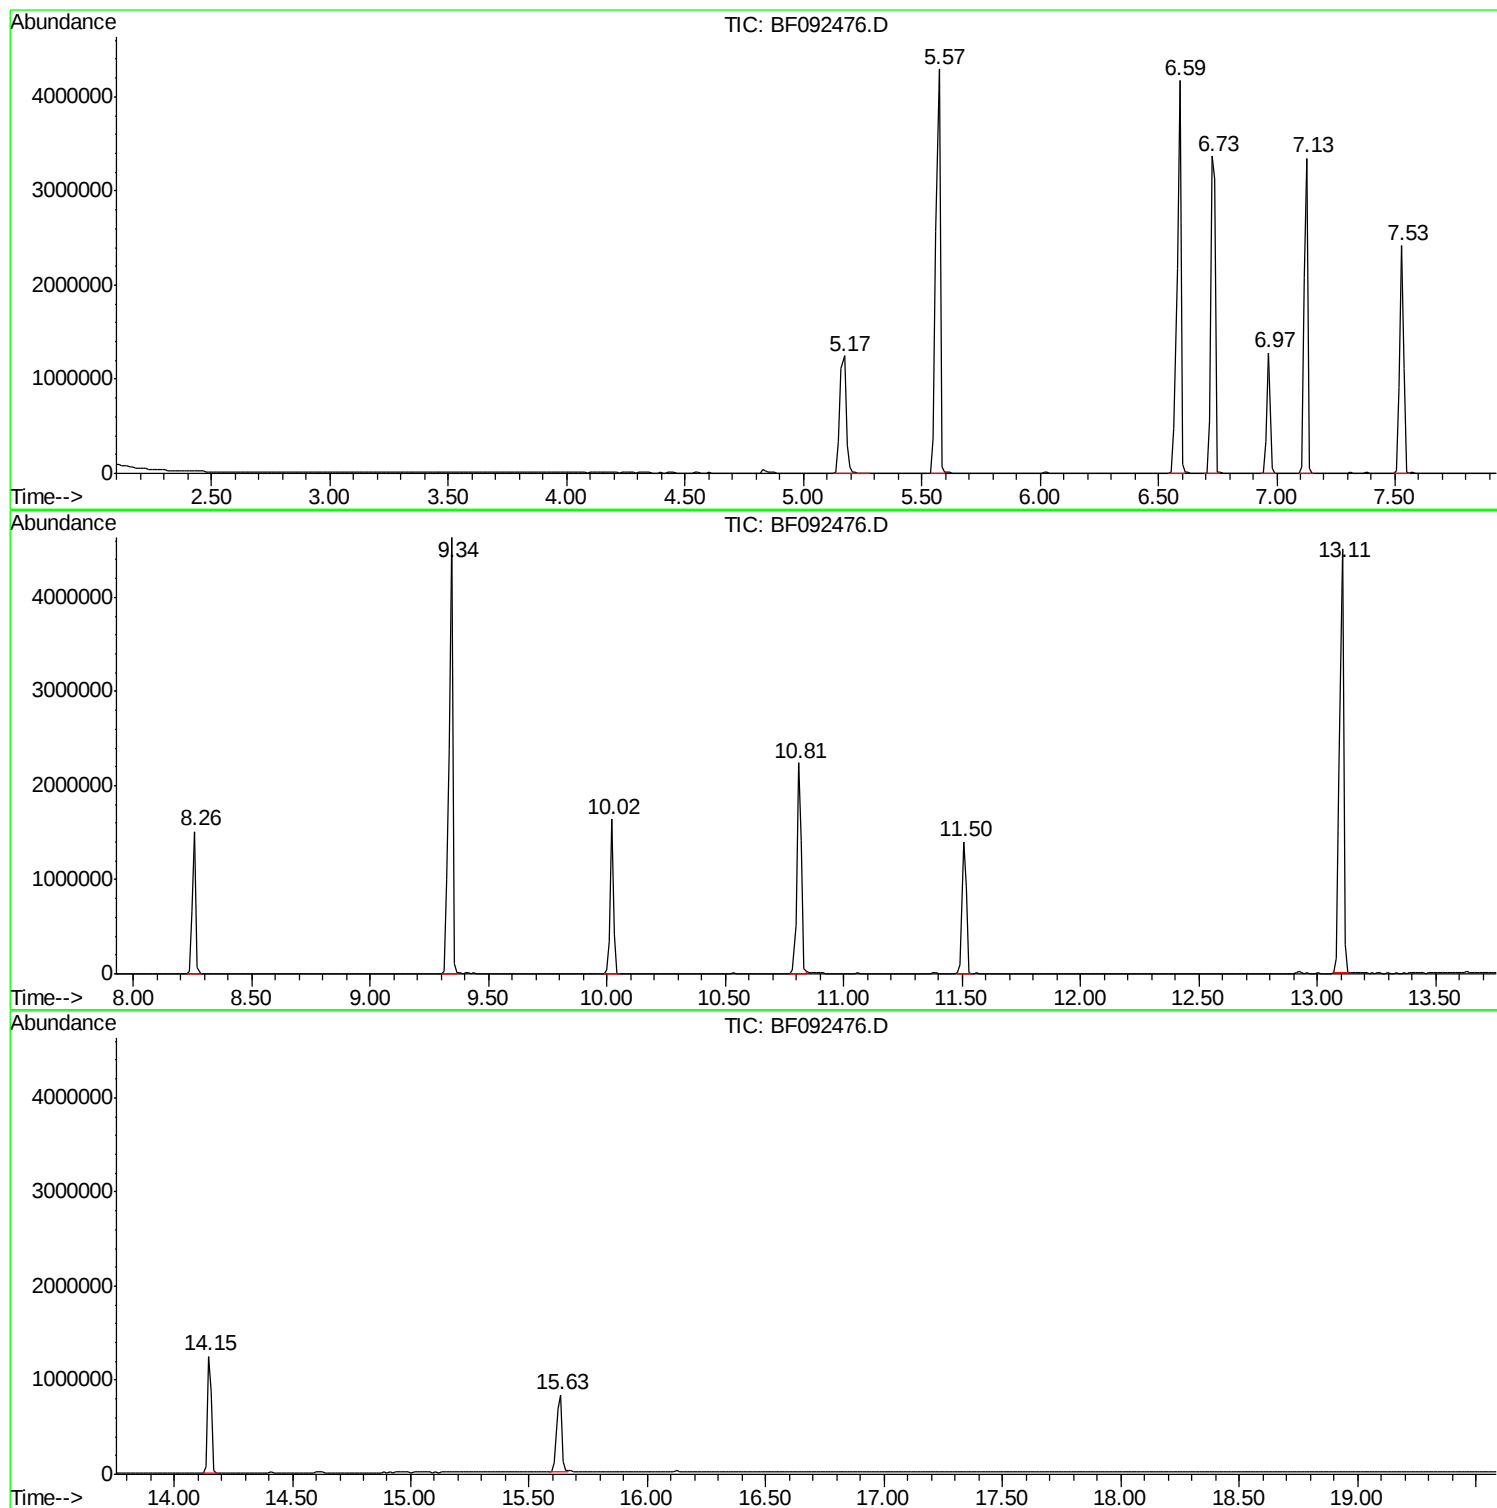

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012517\
Data File : BF092476.D
Acq On : 25 Jan 2017 15:05
Operator : SJ/MA
Sample : PB96241BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96241BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.17	37.12 ng	2115730	1,4-Dichlorobenzene-d4	6.97

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2		Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	25
3		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4		Acetone	58	C3H6O	000067-64-1	9
5		1,2-Butanediol, (.+/-.)-	90	C4H10O2	026171-83-5	9

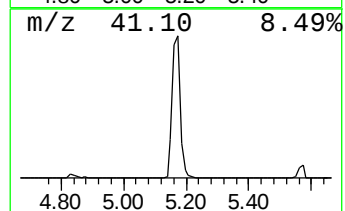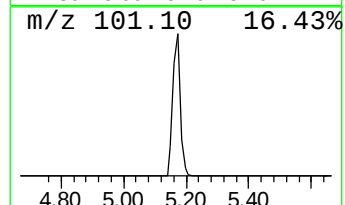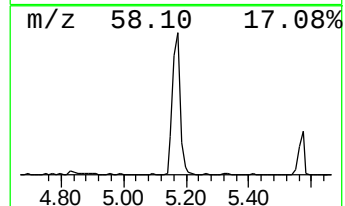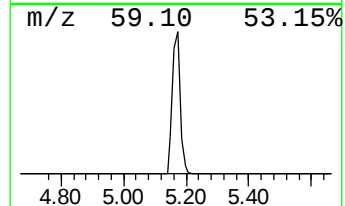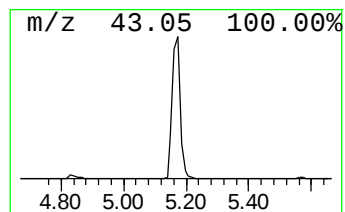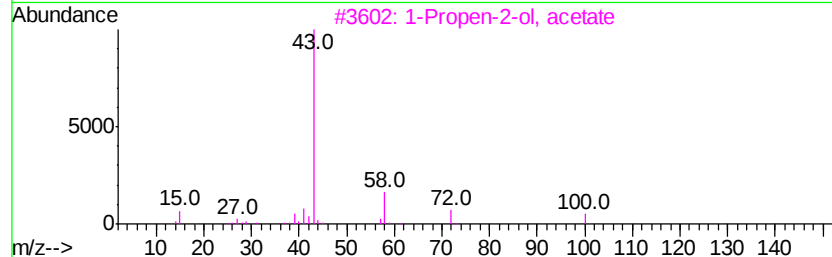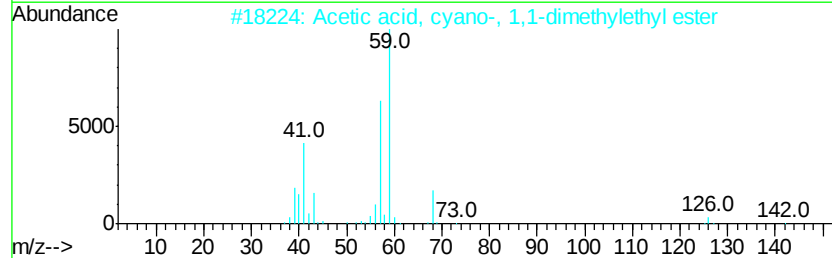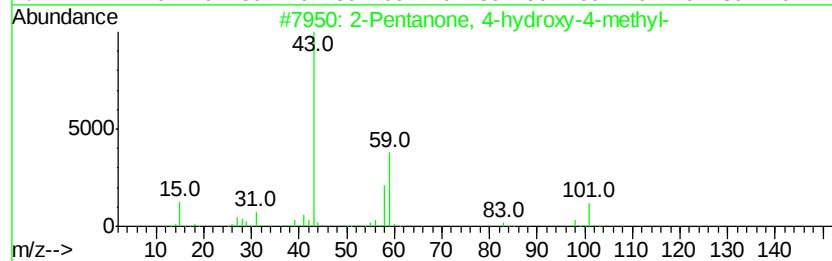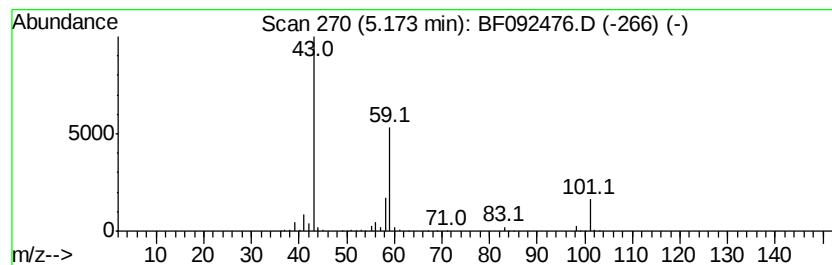

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012517\
Data File : BF092476.D
Acq On : 25 Jan 2017 15:05
Operator : SJ/MA
Sample : PB96241BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96241BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.73 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.73	84.89 ng	4838650	1,4-Dichlorobenzene-d4	6.97

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		Xenon	132	Xe	007440-63-3	9

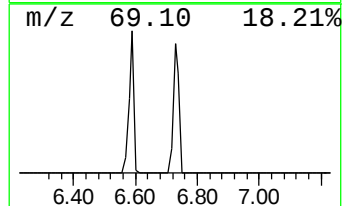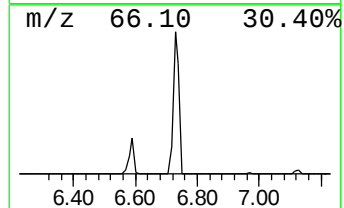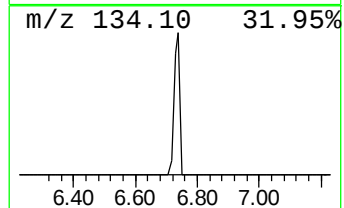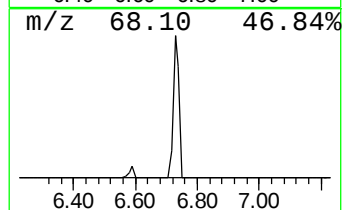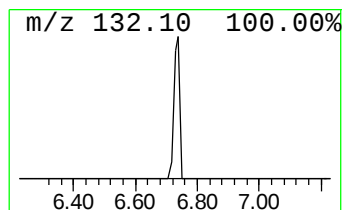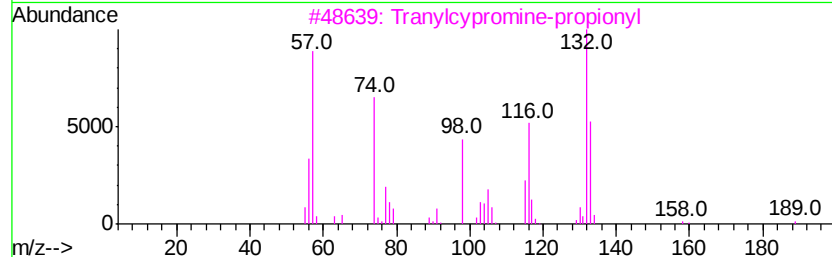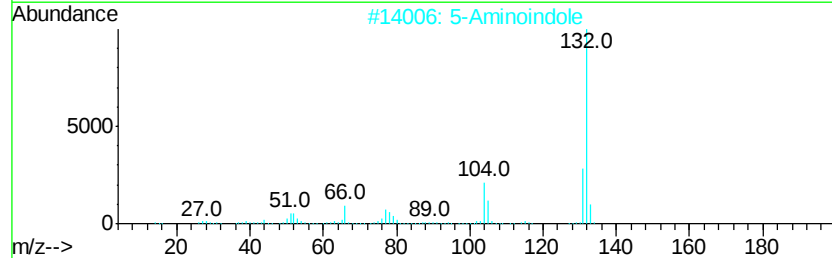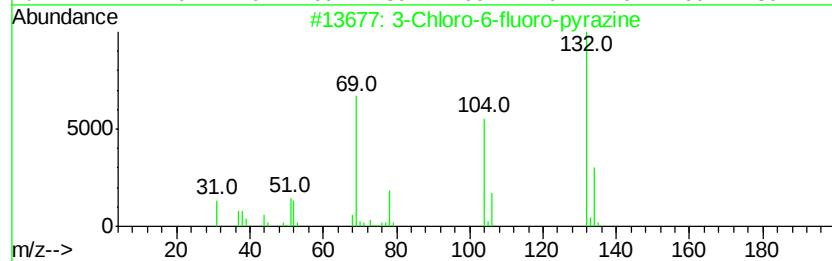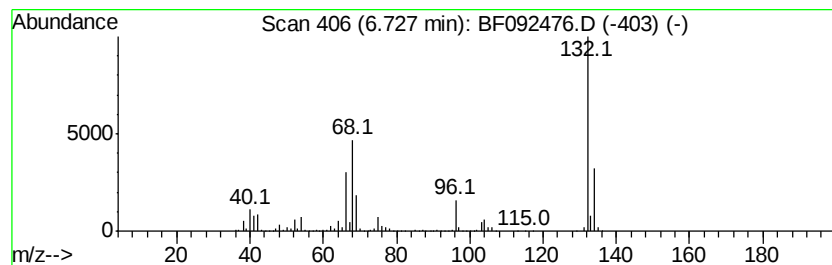

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012517\
Data File : BF092476.D
Acq On : 25 Jan 2017 15:05
Operator : SJ/MA
Sample : PB96241BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96241BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.17	37.1	ng	2115730	1	6.97	1140010	20.0
unknown6.73	6.73	84.9	ng	4838650	1	6.97	1140010	20.0