


Data Path : Z:\HPCHEM1\BNA F\DATA\BF012517\
 Data File : BF092463.D
 Acq On : 25 Jan 2017 9:02
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 24 13:48:07 2017

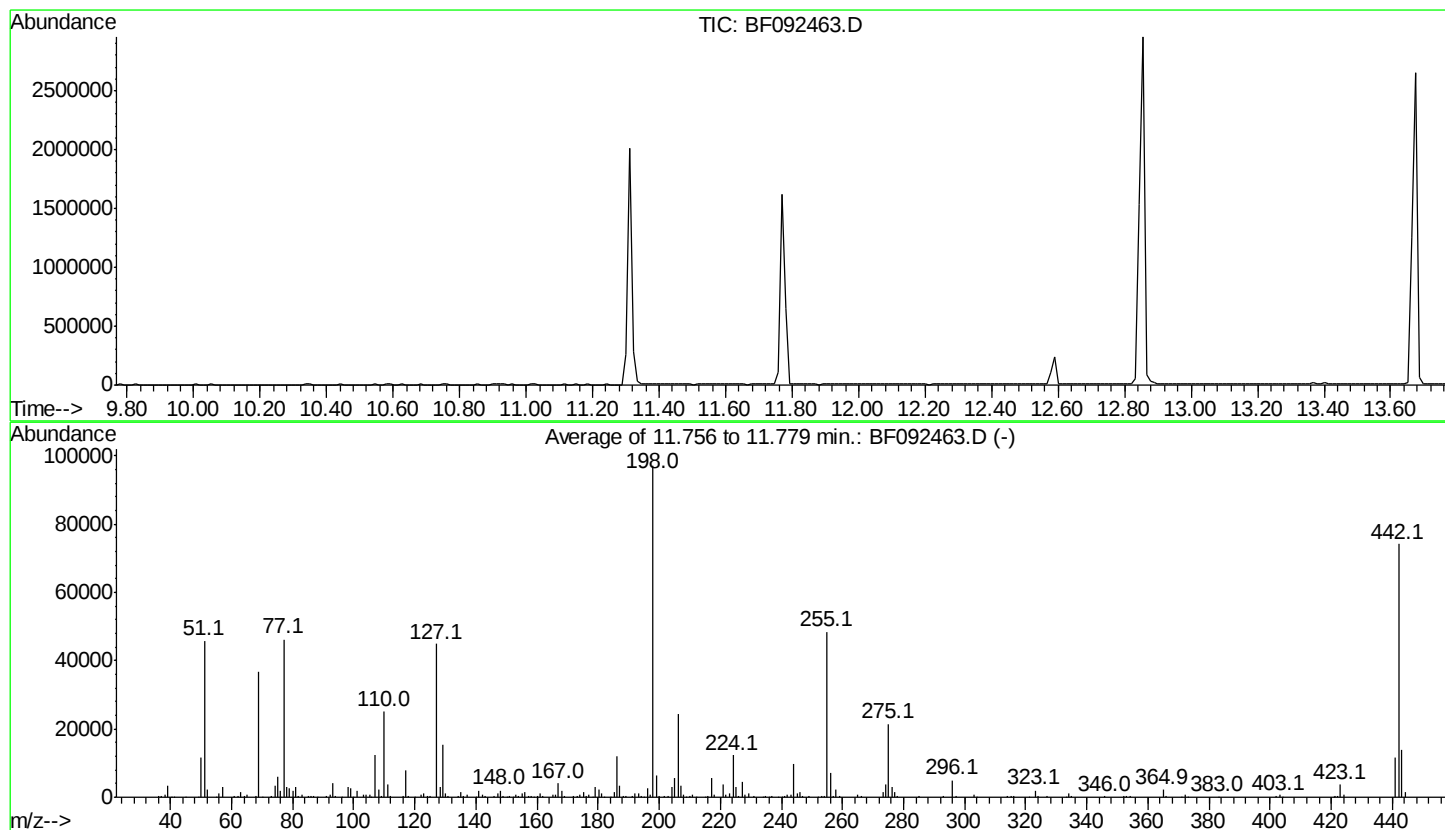

AutoFind: Scans 846, 847, 848; Background Corrected with Scan 843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	45800	PASS
68	69	0.00	2	1.6	573	PASS
69	198	0.00	100	37.9	36836	PASS
70	69	0.00	2	0.4	129	PASS
127	198	10	80	46.2	44911	PASS
197	198	0.00	2	1.0	932	PASS
198	198	100	100	100.0	97142	PASS
199	198	5	9	6.6	6407	PASS
275	198	10	60	22.1	21502	PASS
365	198	1	100	2.3	2237	PASS
441	442	0.01	24	15.5	11515	PASS
442	198	50	100	76.3	74161	PASS
443	442	15	24	18.9	14041	PASS