


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012517\
 Data File : BF092482.D
 Acq On : 25 Jan 2017 17:50
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 24 13:48:07 2017

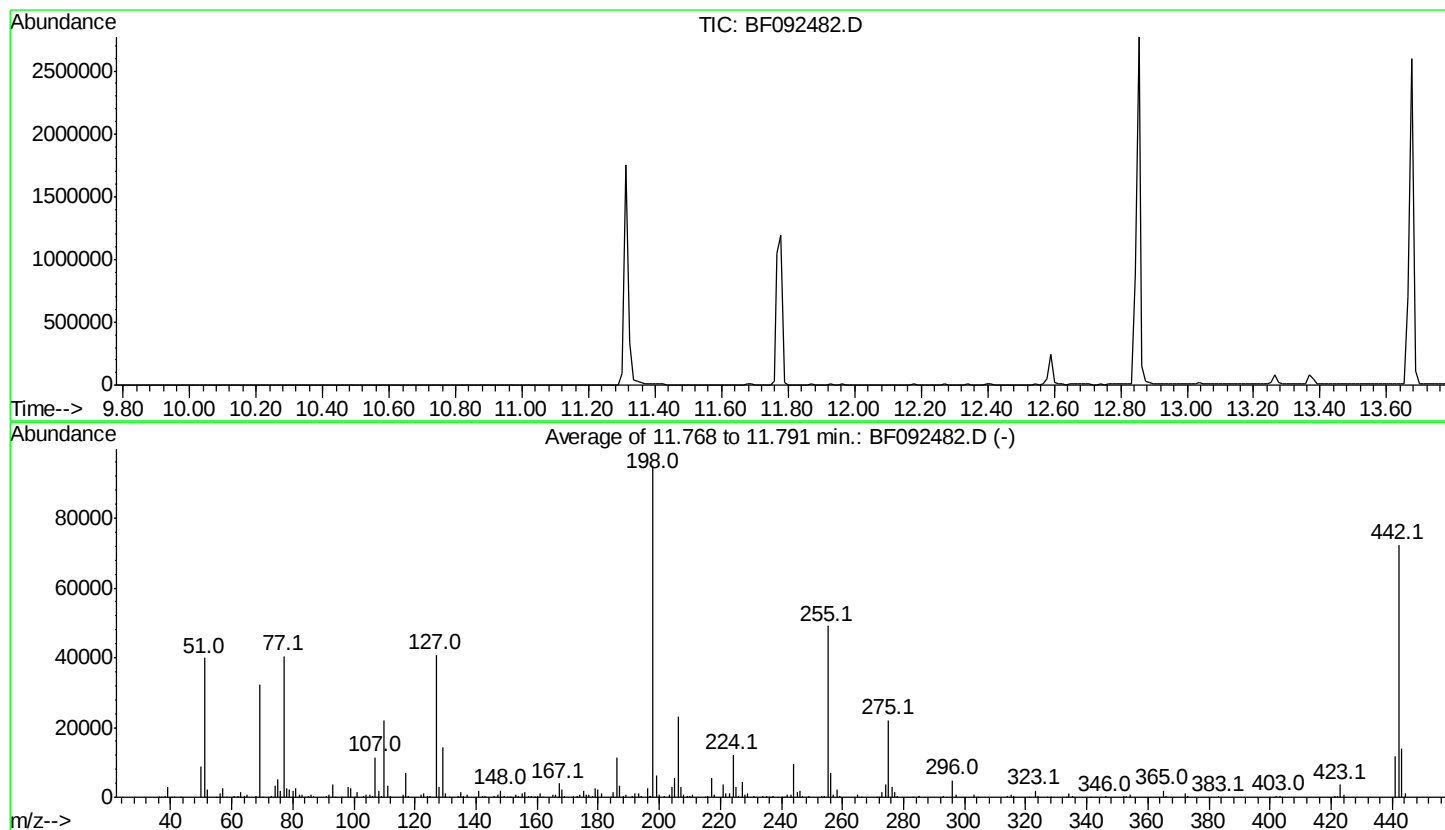

AutoFind: Scans 847, 848, 849; Background Corrected with Scan 843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	39979	PASS
68	69	0.00	2	1.6	519	PASS
69	198	0.00	100	34.1	32397	PASS
70	69	0.00	2	0.3	107	PASS
127	198	10	80	43.0	40874	PASS
197	198	0.00	2	0.5	508	PASS
198	198	100	100	100.0	95074	PASS
199	198	5	9	6.5	6169	PASS
275	198	10	60	23.2	22047	PASS
365	198	1	100	2.1	2008	PASS
441	442	0.01	24	16.2	11735	PASS
442	198	50	100	76.1	72333	PASS
443	442	15	24	19.2	13860	PASS