

Data Path : U:\HPCHEM1\BNA F\DATA\BF012518\
 Data File : BF102453.D
 Acq On : 26 Jan 2018 4:38
 Operator : SJ/JU
 Sample : J1251-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jan 26 05:57:50 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 25 13:44:56 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	134414	20.00	ng	0.00
21) Naphthalene-d8	8.00	136	543973	20.00	ng	0.00
38) Acenaphthene-d10	9.75	164	209782	20.00	ng	0.00
63) Phenanthrene-d10	11.24	188	311031	20.00	ng	0.00
75) Chrysene-d12	13.87	240	273148	20.00	ng	0.00
86) Perylene-d12	15.30	264	215319	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	896014	101.08	ng	0.00
7) Phenol-d6	6.36	99	1072959	100.40	ng	0.00
23) Nitrobenzene-d5	7.29	82	618588	65.35	ng	0.00
41) 2,4,6-Tribromophenol	10.55	330	125341	60.30	ng	0.00
44) 2-Fluorobiphenyl	9.07	172	973556	68.24	ng	0.00
78) Terphenyl-d14	12.82	244	697080	57.53	ng	0.00
Target Compounds						Qvalue
9) Benzaldehyde	6.49	77	18769	2.544	ng	85
10) Phenol	6.37	94	59100	5.065	ng	95
19) n-Nitroso-di-n-propylamine	7.29	70	80768	12.349	ng	# 78
25) Isophorone	7.29	82	618579	36.656	ng	# 64
49) Dimethylphthalate	9.47	163	195493	11.274	ng	100
56) 2,4-Dinitrotoluene	9.75	165	26642	5.795	ng	# 23
66) 4-Bromophenyl-phenylether	10.54	248	8903	2.659	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA F\DATA\BF012518\
Data File : BF102453.D
Acq On : 26 Jan 2018 4:38
Operator : SJ/JU
Sample : J1251-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jan 26 05:57:50 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 25 13:44:56 2018
Response via : Initial Calibration

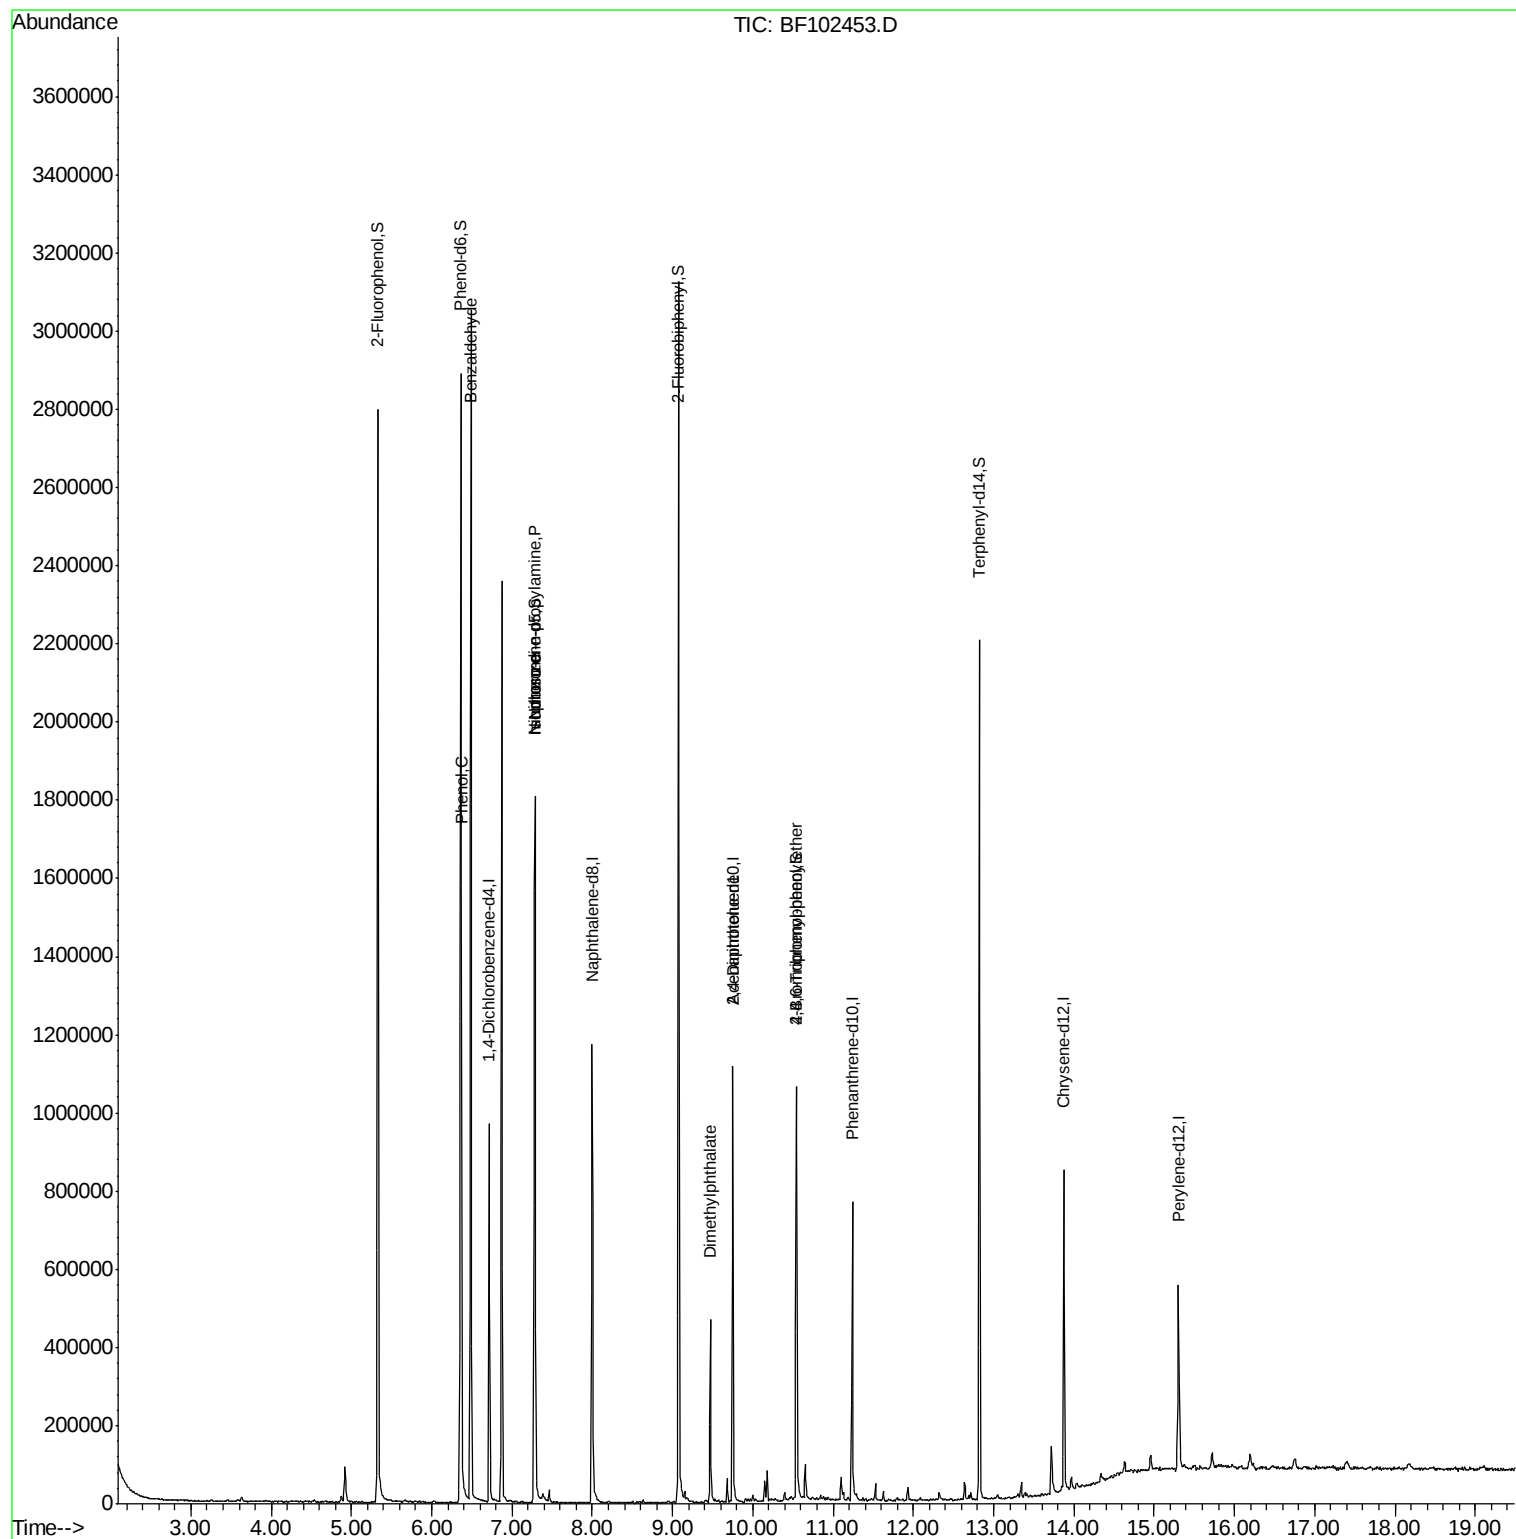

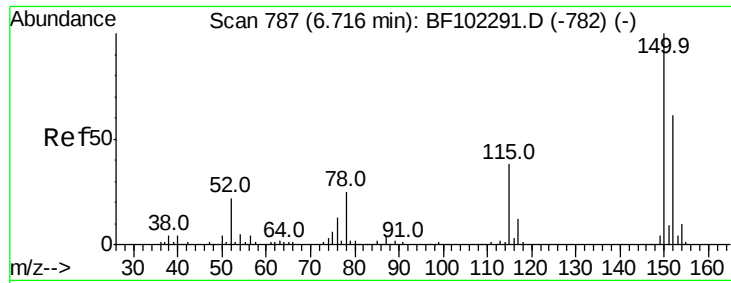


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.72 min Scan# 787
Delta R.T. 0.00 min
Lab File: BF102453.D
Acq: 26 Jan 2018 4:38

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.8	124.6	186.8
115	61.4	50.1	75.1

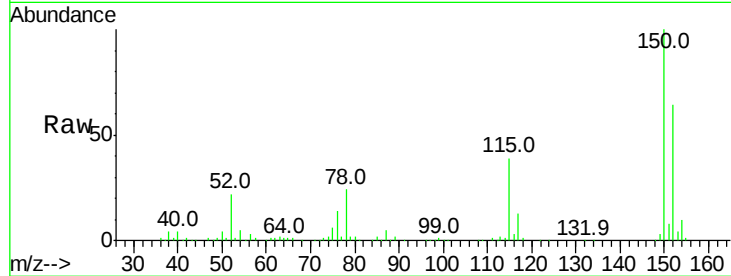


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

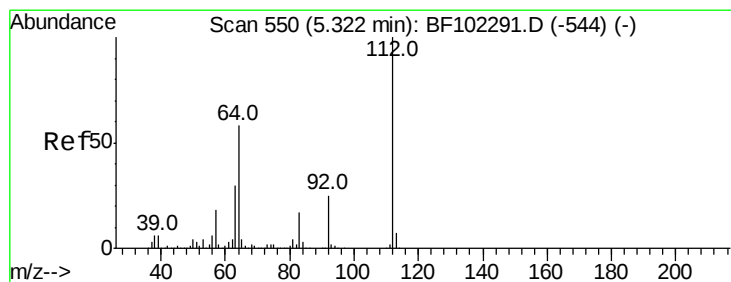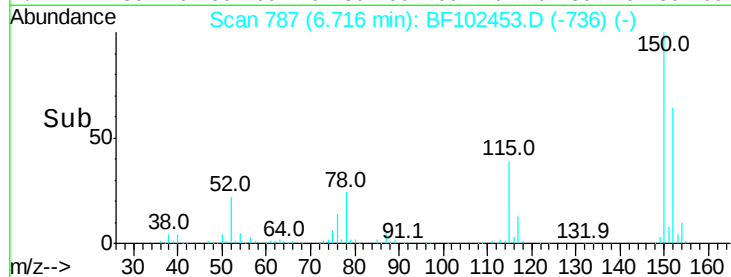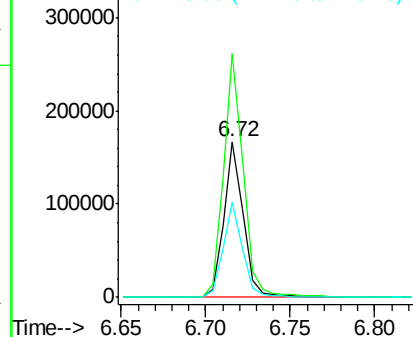



#5


2-Fluorophenol
Concen: 101.075 ng
RT: 5.33 min Scan# 551
Delta R.T. 0.01 min
Lab File: BF102453.D
Acq: 26 Jan 2018 4:38

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.8	47.9	71.9
63	31.3	23.7	35.5

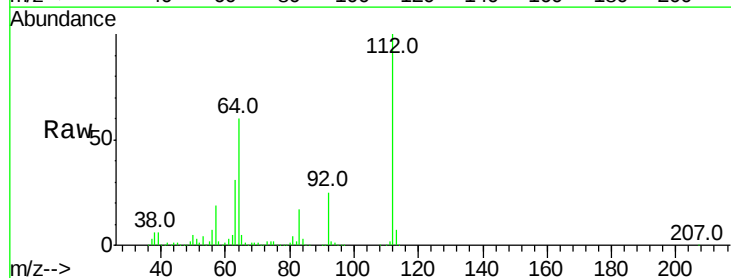

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

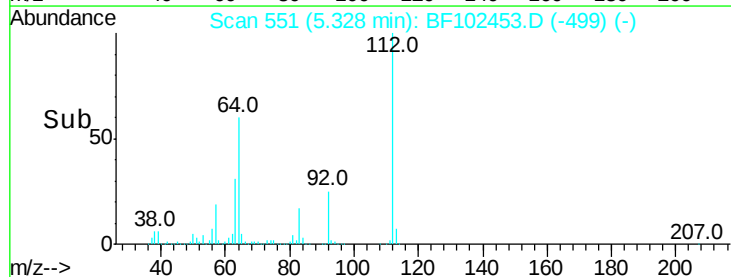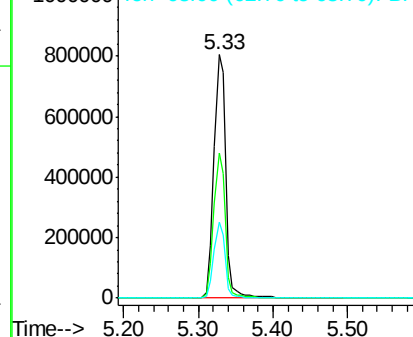

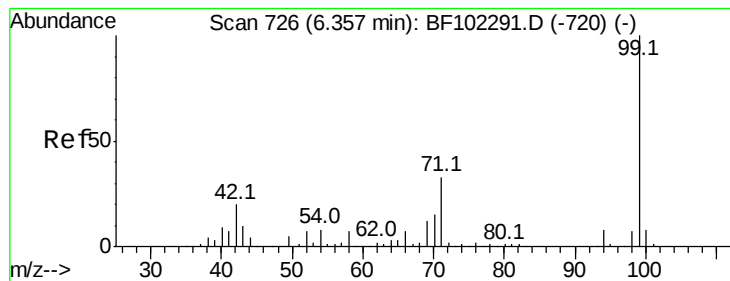

#7

Phenol-d6

Concen: 100.395 ng

RT: 6.36 min Scan# 727

Delta R.T. -0.01 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 1072959

Ion Ratio Lower Upper




99 100

42 19.4 14.5 21.7

71 34.9 25.4 38.0

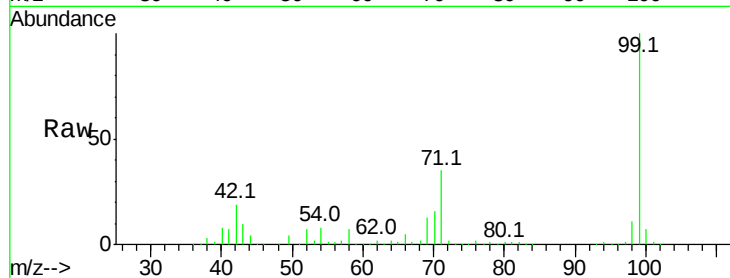

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

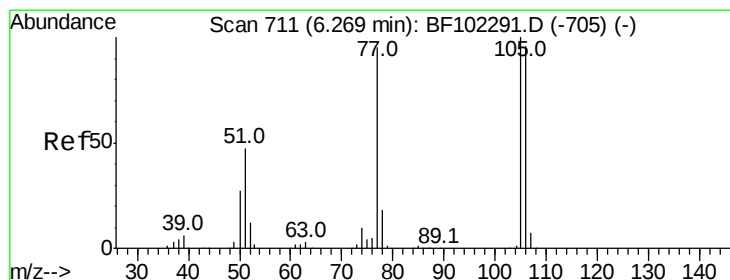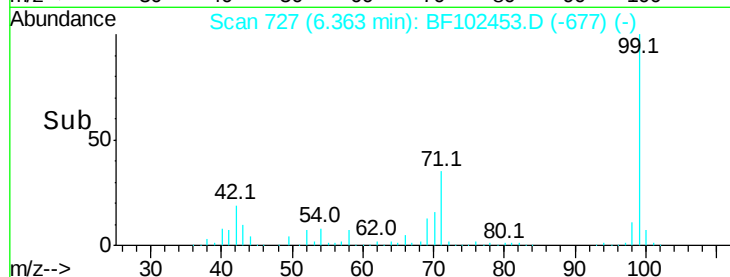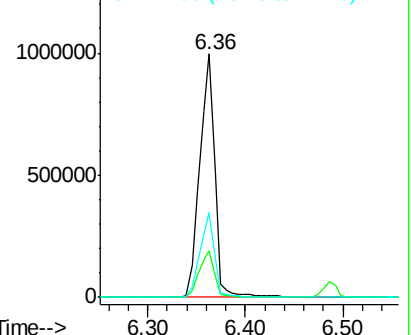

#9

Benzaldehyde

Concen: 2.544 ng

RT: 6.49 min Scan# 748

Delta R.T. 0.22 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38


Tgt Ion: 77 Resp: 18769

Ion Ratio Lower Upper



77 100


105 84.7 81.1 121.1

106 80.8 74.5 114.5

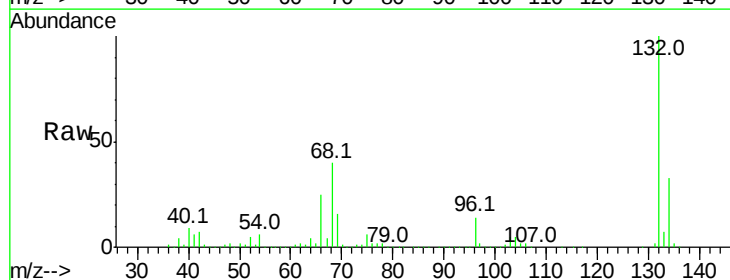

Abundance Ion 77.00 (76.70 to 77.70): BF1
Ion 105.00 (104.70 to 105.70): BF1
Ion 106.00 (105.70 to 106.70): BF1

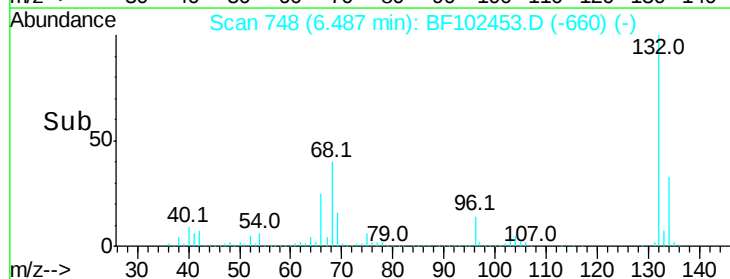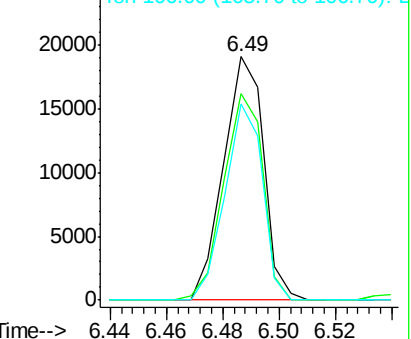

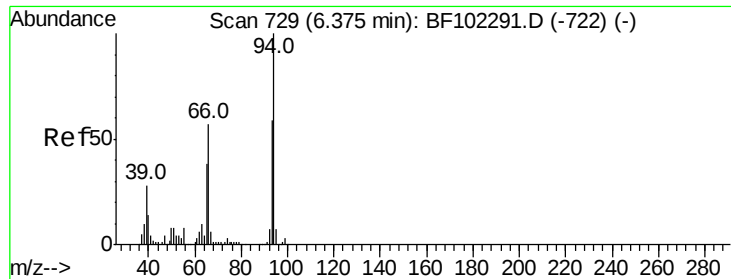

#10

Phenol

Concen: 5.065 ng

RT: 6.37 min Scan# 729

Delta R.T. -0.01 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38

Instrument :

BNA_F

ClientSampled :





Tot Ion: 94 Resp: 59100

Ion Ratio Lower Upper

94 100

65 24.8 7.9 47.9

66 33.1 16.2 56.2

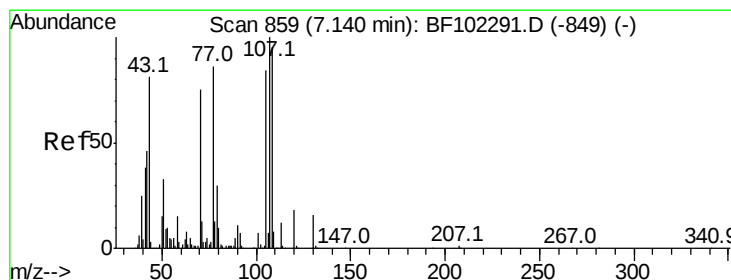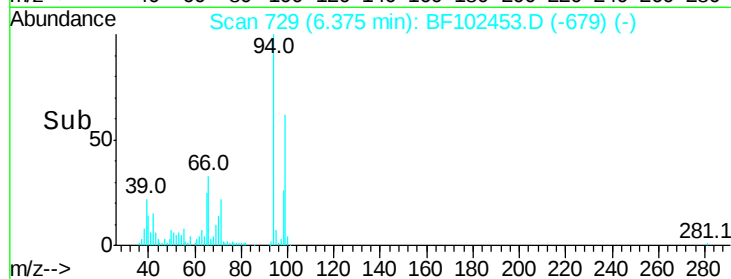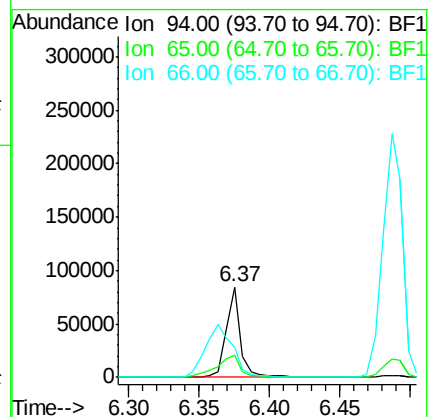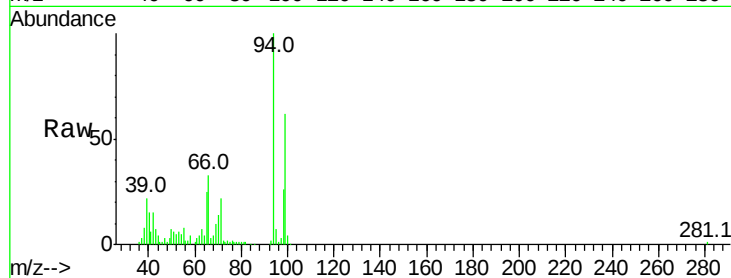

#19

n-Nitroso-di-n-propylamine

Concen: 12.349 ng

RT: 7.29 min Scan# 884

Delta R.T. 0.14 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38

Tgt Ion: 70 Resp: 80768




Ion Ratio Lower Upper


70 100

42 48.4 47.5 71.3

101 0.0 7.4 11.2#

130 2.1 16.6 25.0#

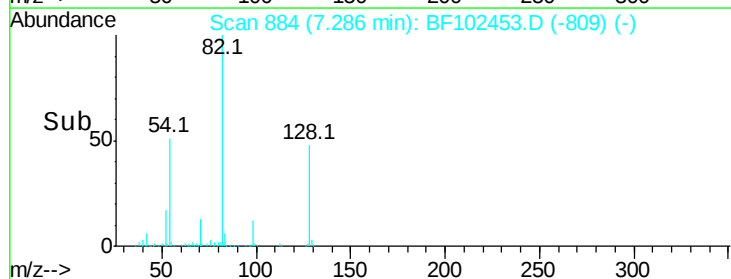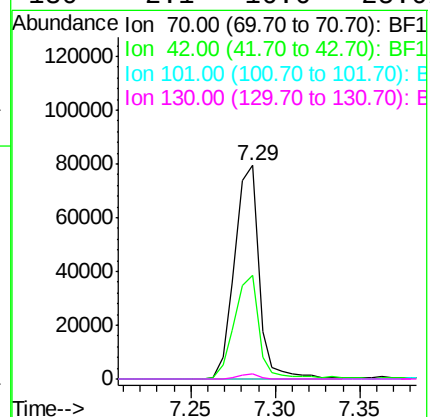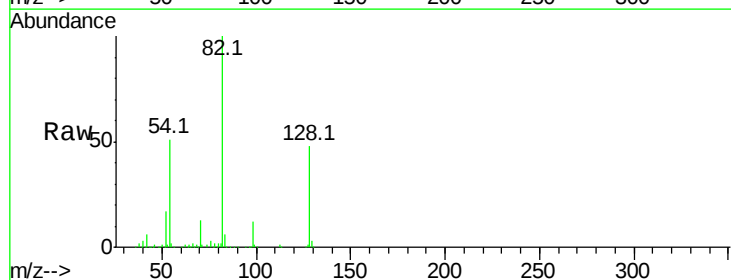

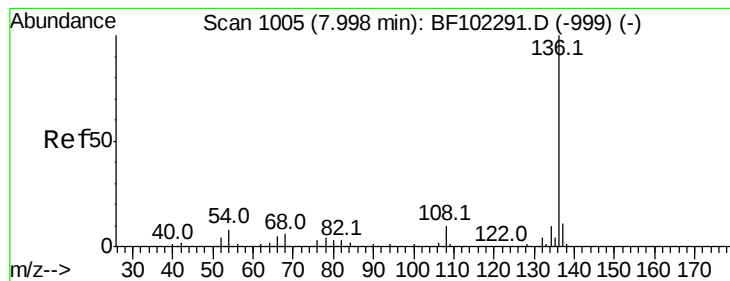

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.00 min Scan# 1005

Delta R.T. 0.00 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 543973


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 7.9 6.6 9.8

68 5.3 5.0 7.4



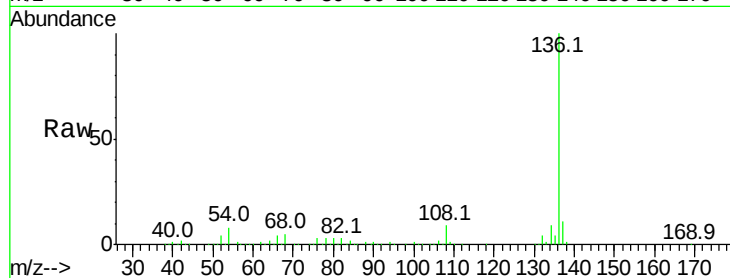


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

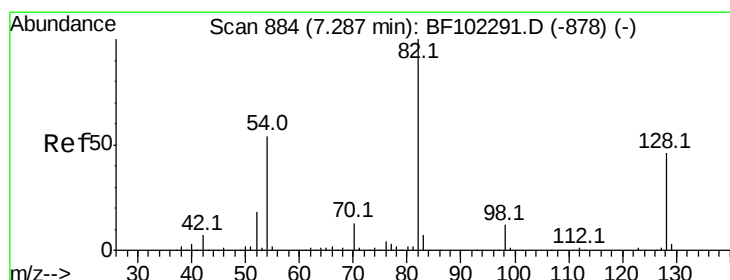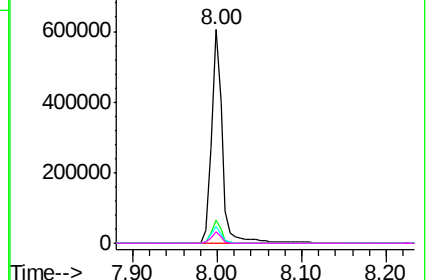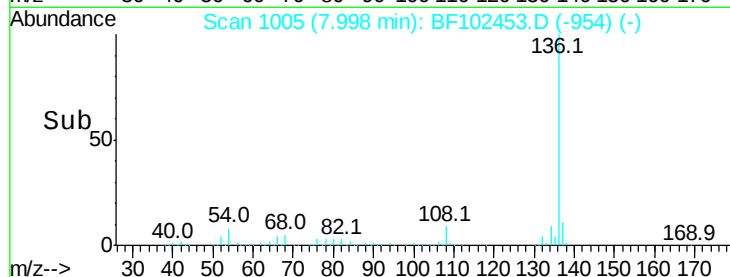

#23

Nitrobenzene-d5

Concen: 65.349 ng

RT: 7.29 min Scan# 884

Delta R.T. -0.01 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38


Tgt Ion: 82 Resp: 618588

Ion Ratio Lower Upper

82 100

128 47.8 36.1 54.1



54 51.0 41.4 62.2

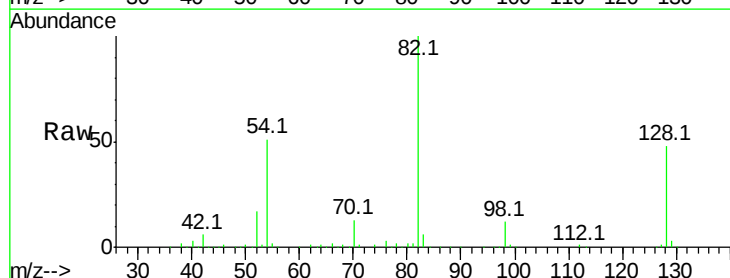


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

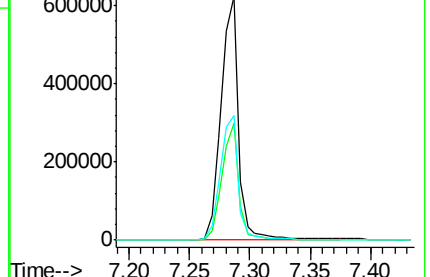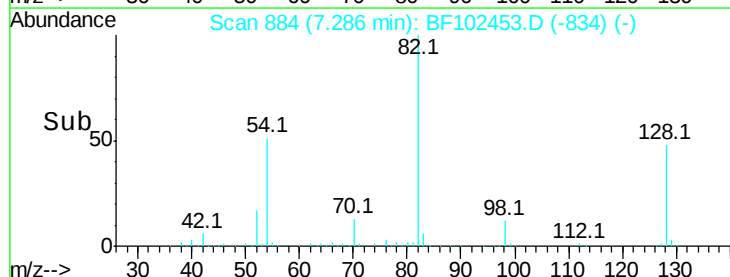

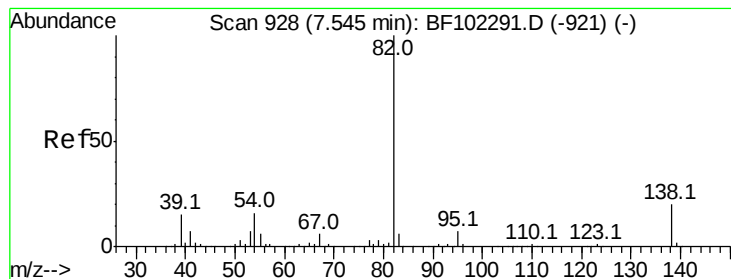

#25

Isophorone

Concen: 36.656 ng

RT: 7.29 min Scan# 884

Delta R.T. -0.26 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 618579

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

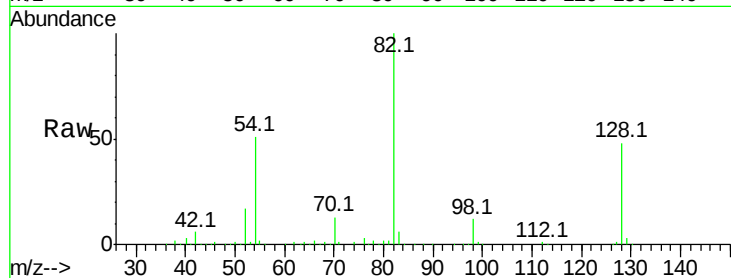

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

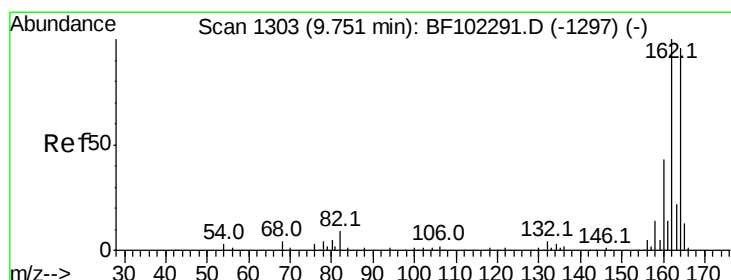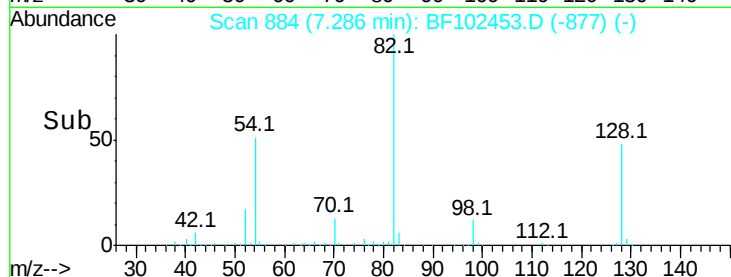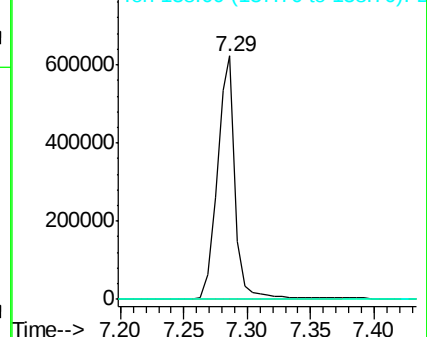

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.75 min Scan# 1303

Delta R.T. -0.01 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38


Tgt Ion:164 Resp: 209782

Ion Ratio Lower Upper



164 100


162 102.3 86.1 129.1

160 45.2 38.3 57.5

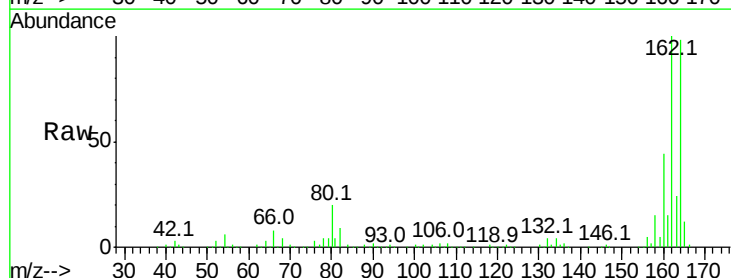

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

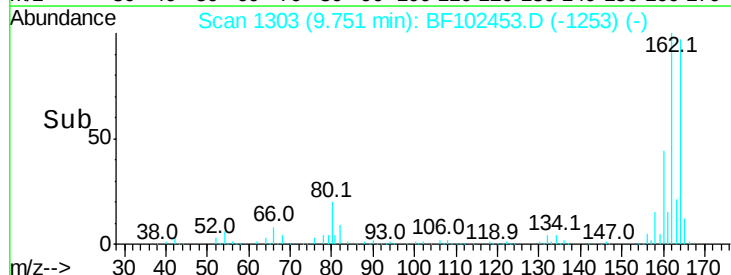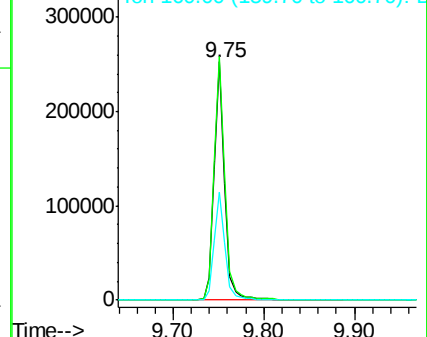


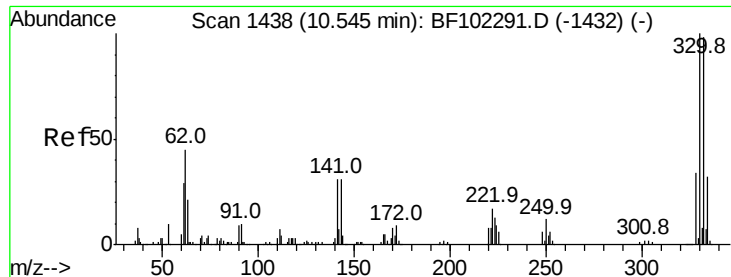




#41
 2,4,6-Tribromophenol
 Concen: 60.300 ng
 RT: 10.55 min Scan# 1438
 Delta R.T. 0.00 min
 Lab File: BF102453.D
 Acq: 26 Jan 2018 4:38

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.7	77.0	115.6
141	41.9	29.9	44.9

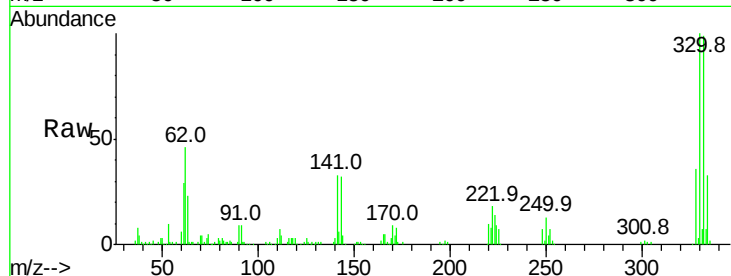


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

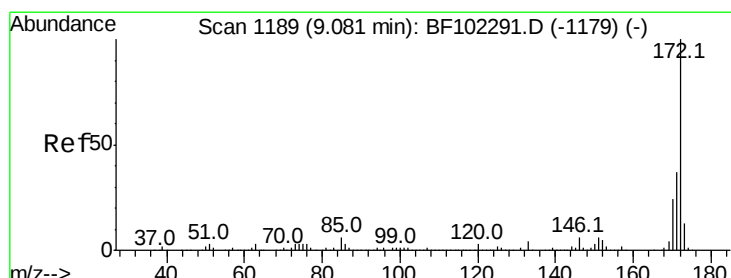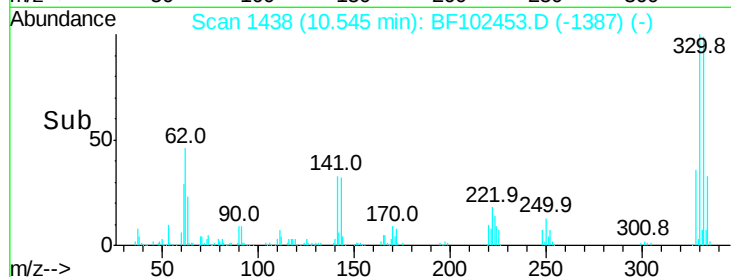
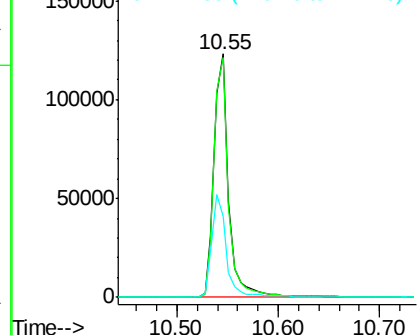



#44
 2-Fluorobiphenyl
 Concen: 68.236 ng
 RT: 9.07 min Scan# 1188
 Delta R.T. -0.01 min
 Lab File: BF102453.D
 Acq: 26 Jan 2018 4:38

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.8	29.7	44.5
170	24.6	19.6	29.4

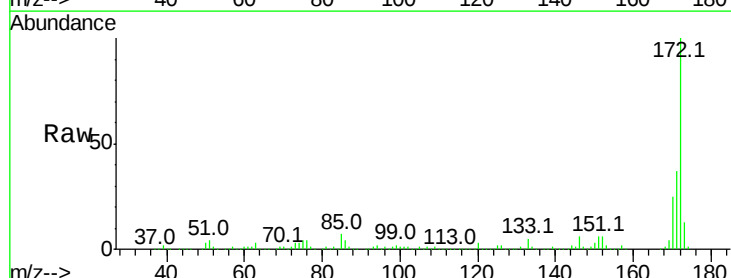

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

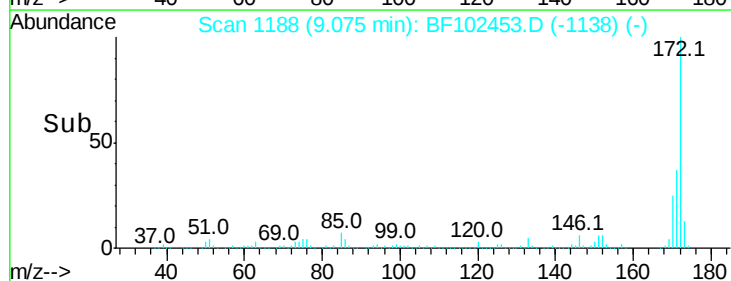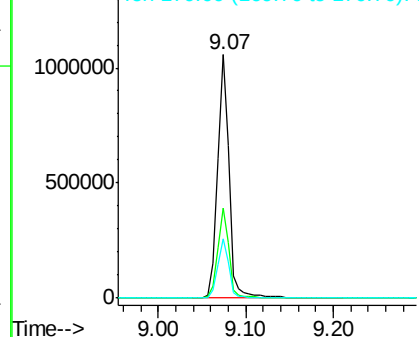

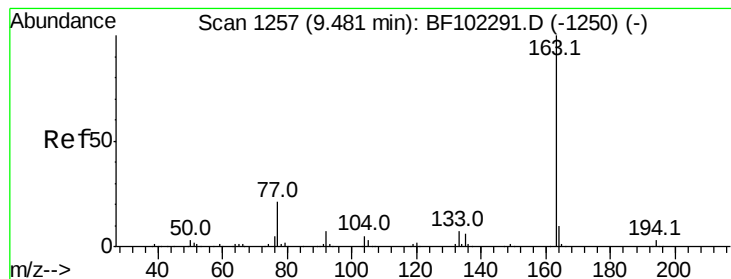

#49

Dimethylphthalate

Concen: 11.274 ng

RT: 9.47 min Scan# 1255

Delta R.T. -0.02 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38

Instrument :

BNA_F

ClientSampled :


Tot Ion:163 Resp: 195493

Ion Ratio Lower Upper

163 100

194 3.3 2.7 4.1




164 10.1 8.2 12.2

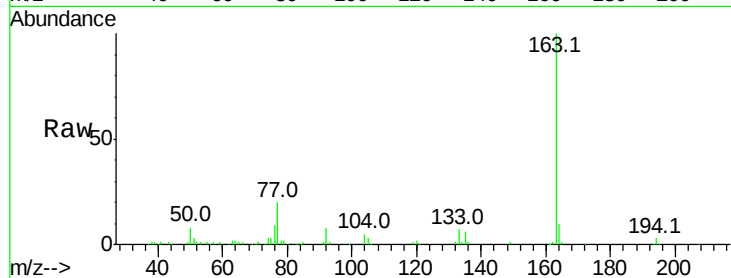

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

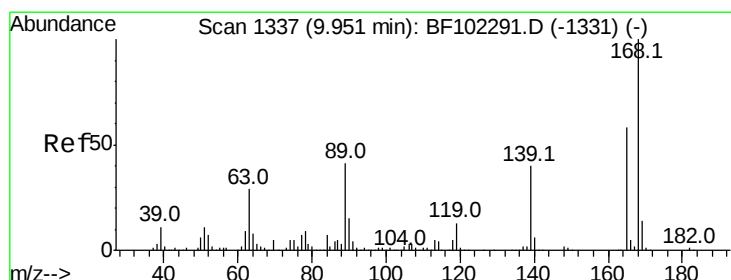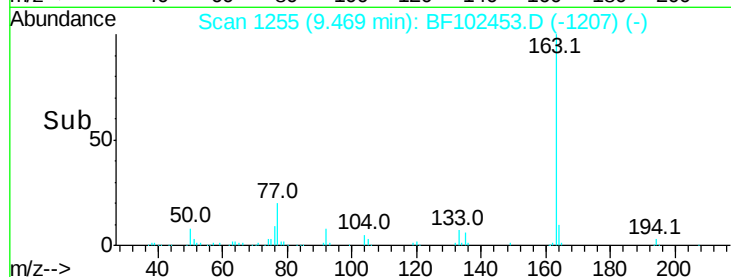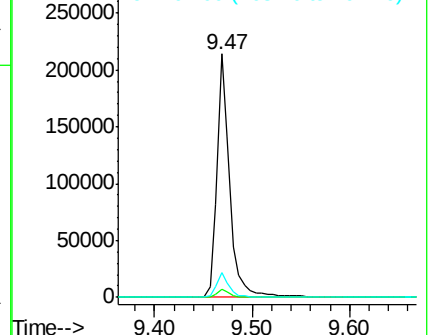

#56

2,4-Dinitrotoluene

Concen: 5.795 ng

RT: 9.75 min Scan# 1303

Delta R.T. -0.21 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38

Tgt Ion:165 Resp: 26642


Ion Ratio Lower Upper

165 100

63 1.1 36.4 54.6#

89 1.7 57.8 86.6#

182 0.0 1.6 2.4#


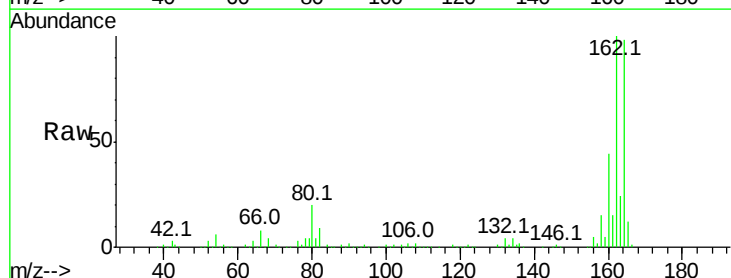



Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E



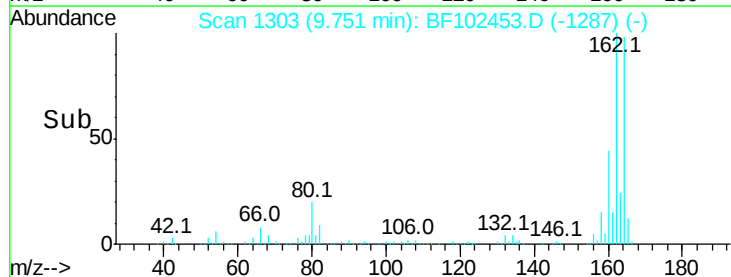
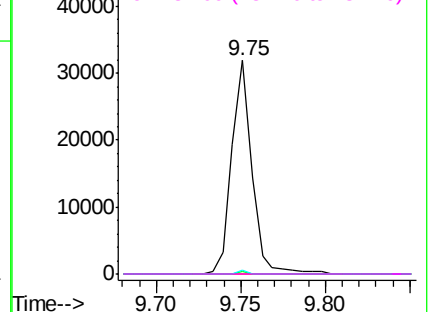


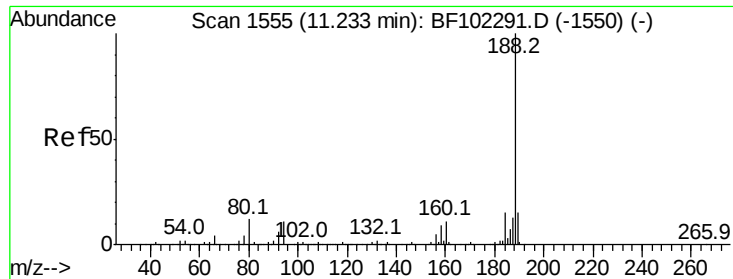

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.24 min Scan# 1556
Delta R.T. 0.00 min
Lab File: BF102453.D
Acq: 26 Jan 2018 4:38




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 311031
Ion Ratio Lower Upper
188 100
94 9.7 8.5 12.7
80 10.4 9.2 13.8

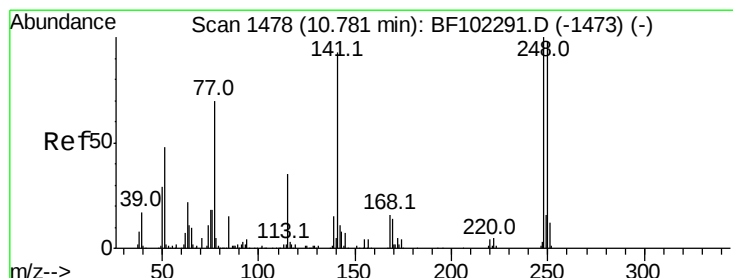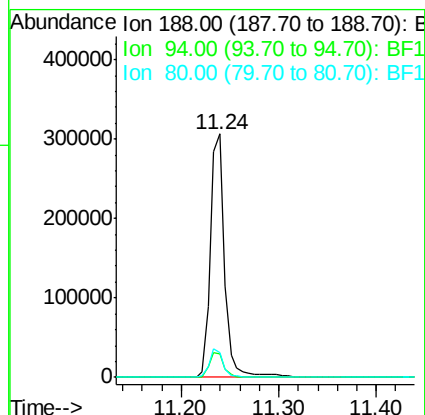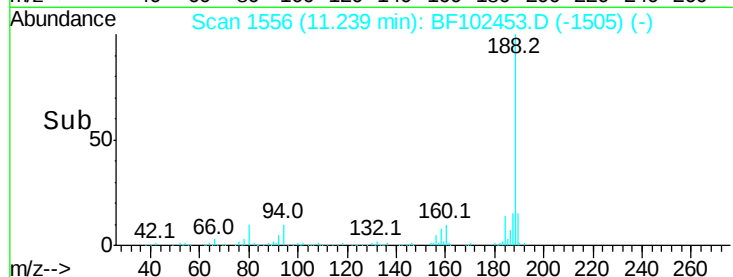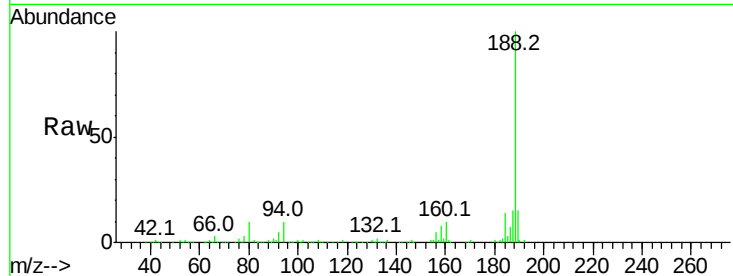

#66
4-Bromophenyl-phenylether
Concen: 2.659 ng
RT: 10.54 min Scan# 1437
Delta R.T. -0.25 min
Lab File: BF102453.D
Acq: 26 Jan 2018 4:38

Tgt Ion:248 Resp: 8903
Ion Ratio Lower Upper
248 100
250 195.2 76.9 115.3#
141 602.7 74.4 111.6#

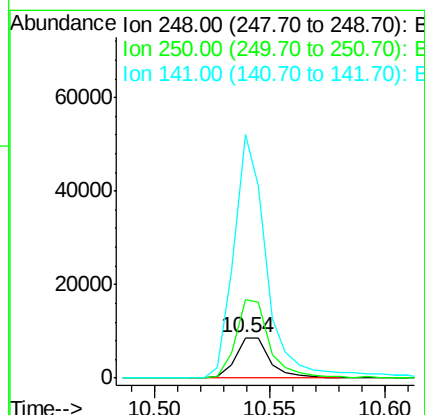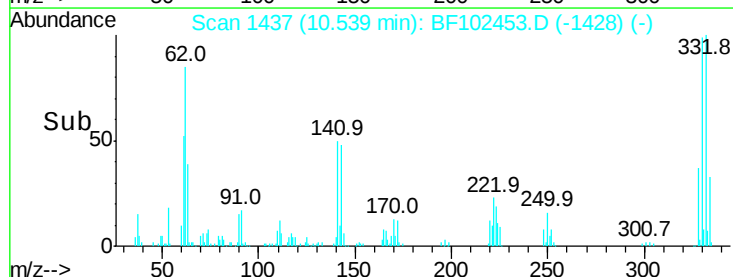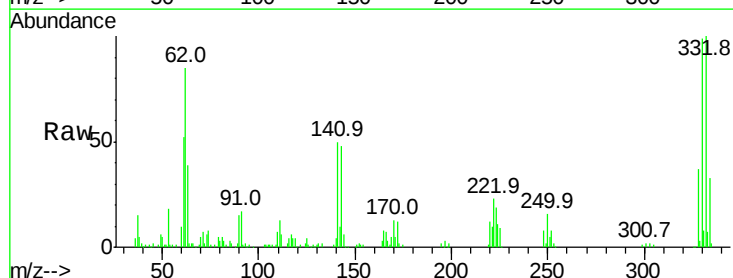

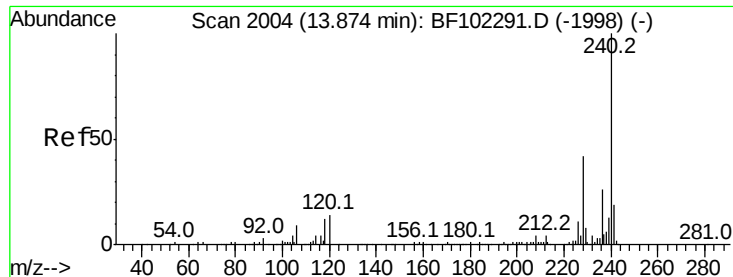

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.87 min Scan# 2004

Delta R.T. -0.01 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 273148

Ion Ratio Lower Upper

240 100

120 14.4 9.5 14.3#




236 25.8 20.7 31.1

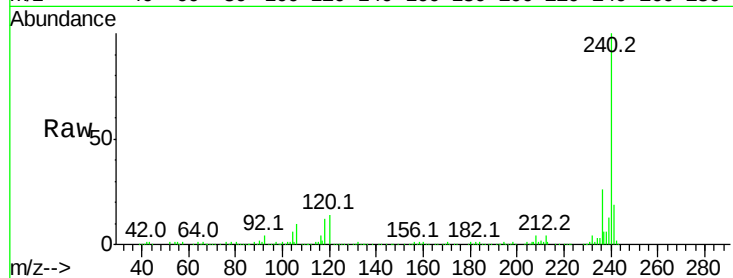

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

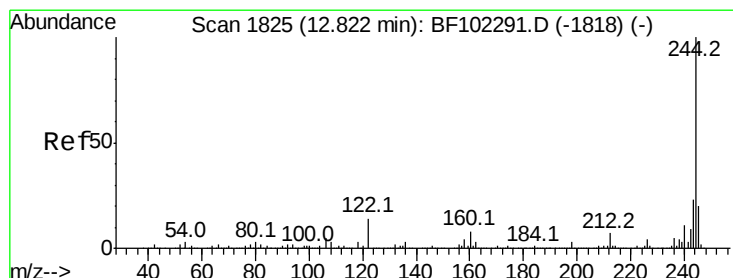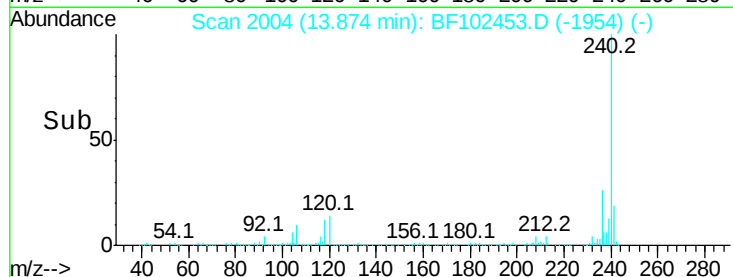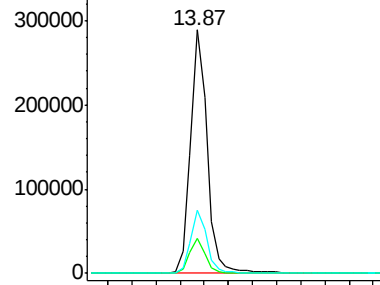

#78

Terphenyl-d14

Concen: 57.532 ng

RT: 12.82 min Scan# 1825

Delta R.T. -0.01 min

Lab File: BF102453.D

Acq: 26 Jan 2018 4:38


Tgt Ion:244 Resp: 697080

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.0



122 14.5 11.0 16.4

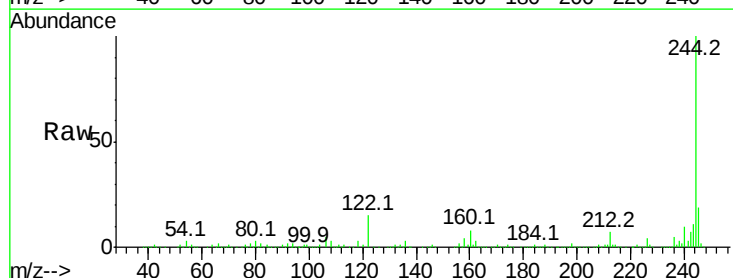


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

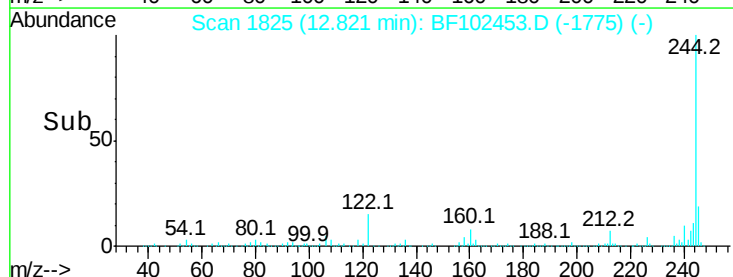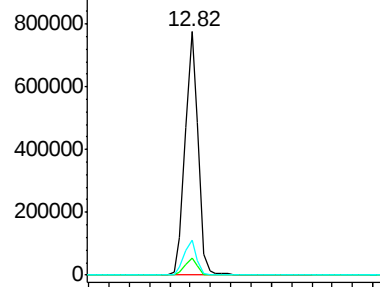


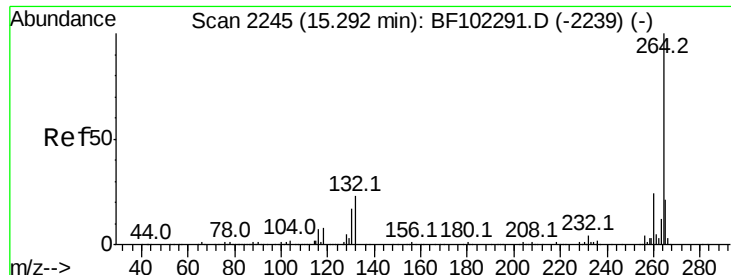

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.30 min Scan# 2247
Delta R.T. 0.01 min
Lab File: BF102453.D
Acq: 26 Jan 2018 4:38

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.2	28.8
265	21.1	17.5	26.3

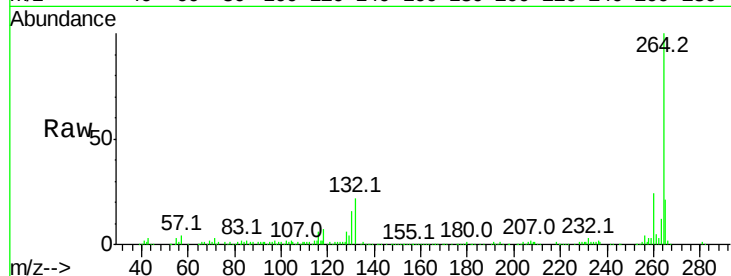

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

