
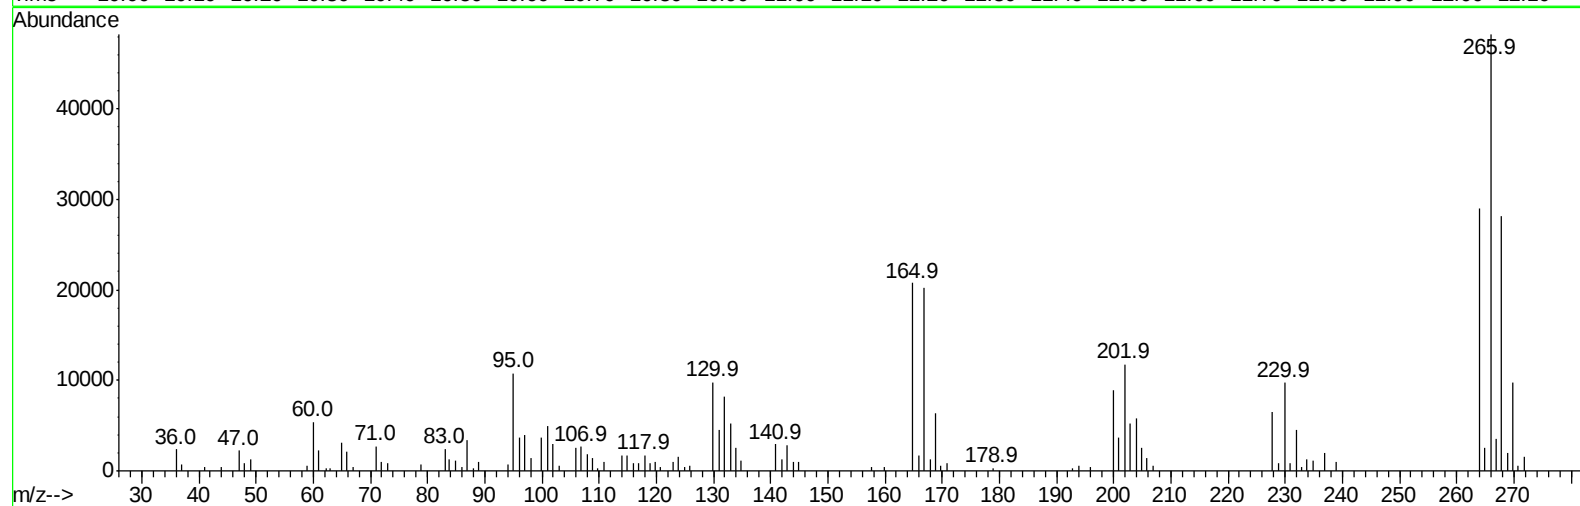


Data Path : U:\HPCHEM1\BNA F\DATA\BF012518\
Data File : BF102430.D
Acq On : 25 Jan 2018 17:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 04:25:52 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 25 13:44:56 2018
Response via : Initial Calibration

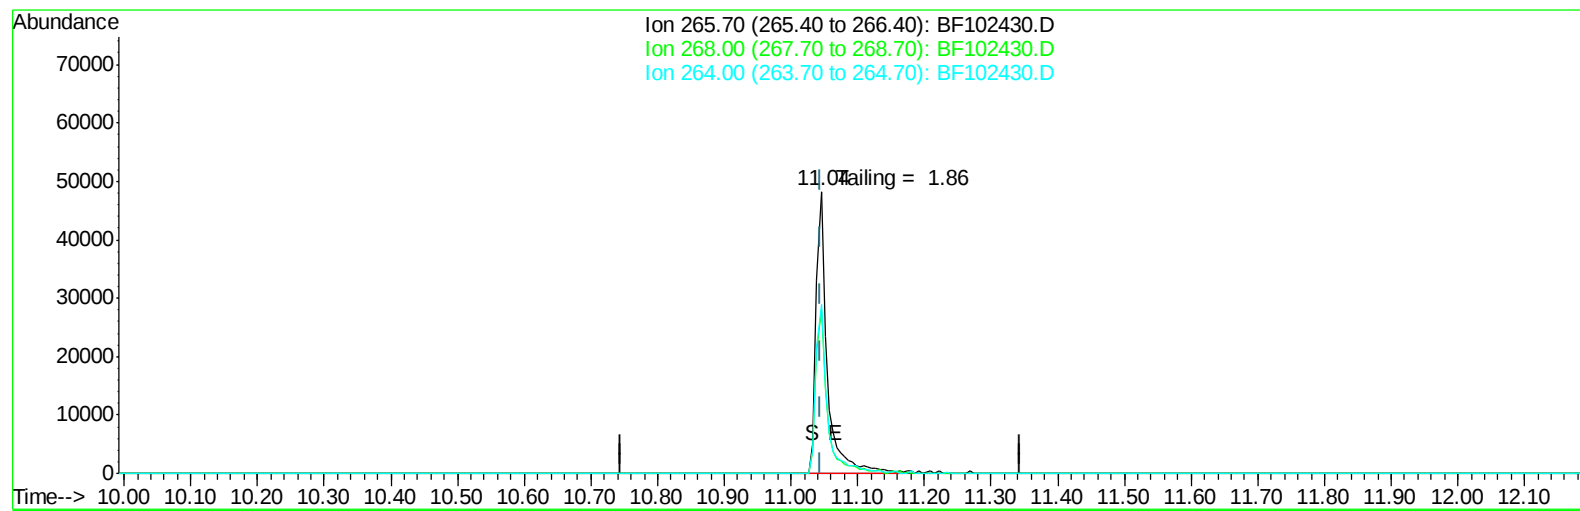

TIC: BF102430.D

(69) Pentachlorophenol (C)



11.045min (-0.000) 66233.34ng

response 54037

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.42
264.00	61.90	60.18
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF012518\
Data File : BF102430.D
Acq On : 25 Jan 2018 17:25
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 04:25:52 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 25 13:44:56 2018
Response via : Initial Calibration

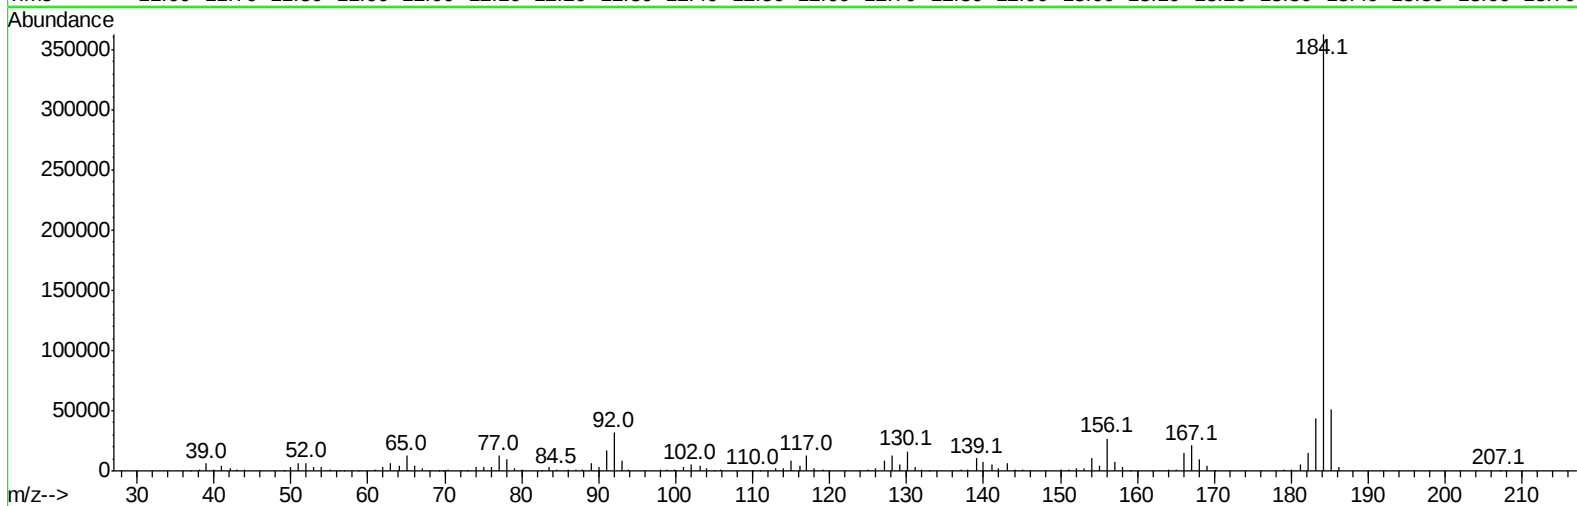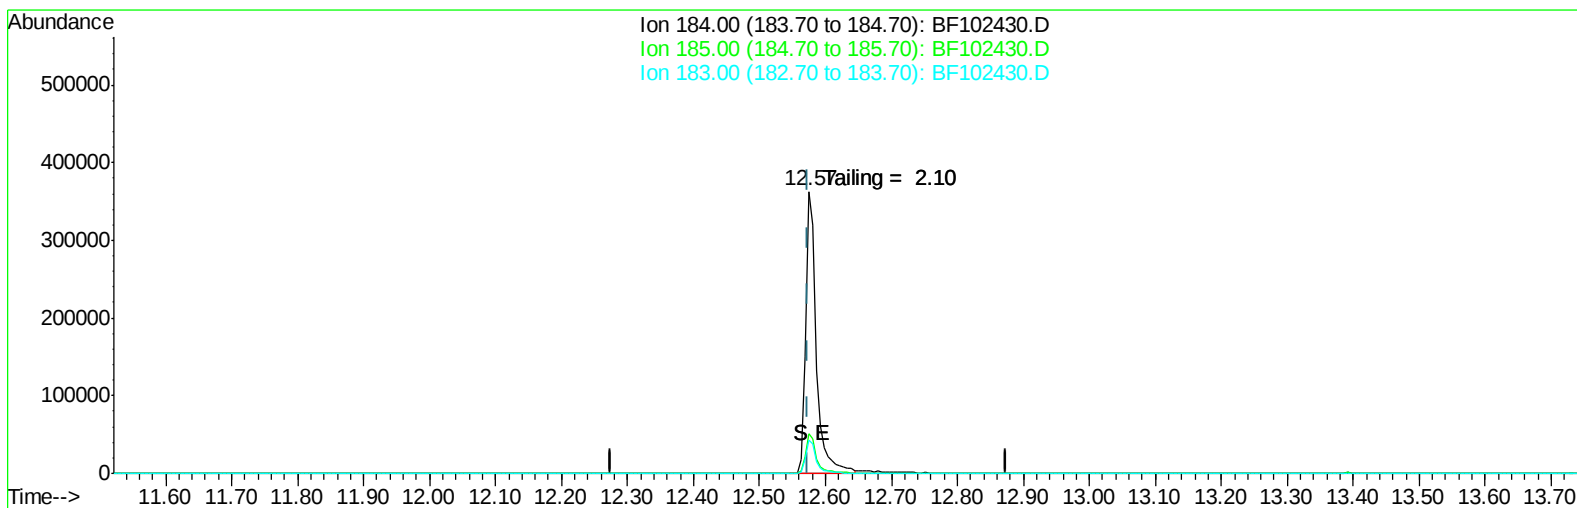

TIC: BF102430.D

(76) Benzidine

12.574min (-0.000) 0.00ng m

response 413283

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.99
183.00	11.60	12.04
0.00	0.00	0.00