
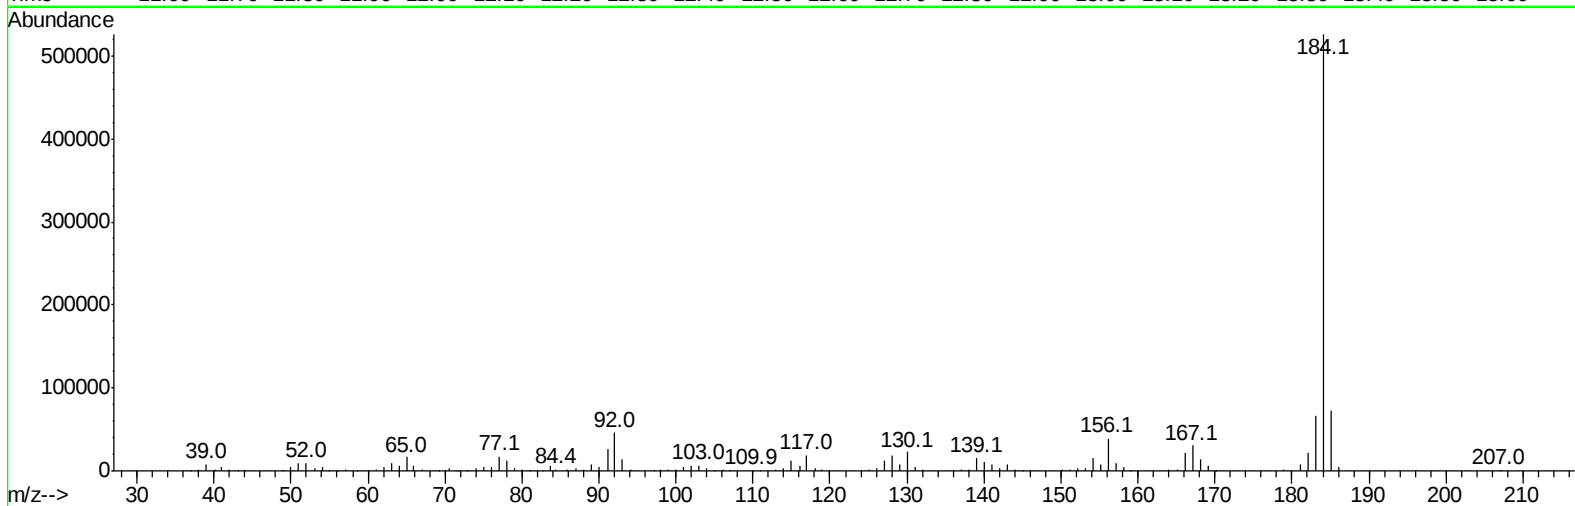


Data Path : U:\HPCHEM1\BNA F\DATA\BF012518\
 Data File : BF102414.D
 Acq On : 25 Jan 2018 9:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 04:22:40 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 25 13:44:56 2018
 Response via : Initial Calibration

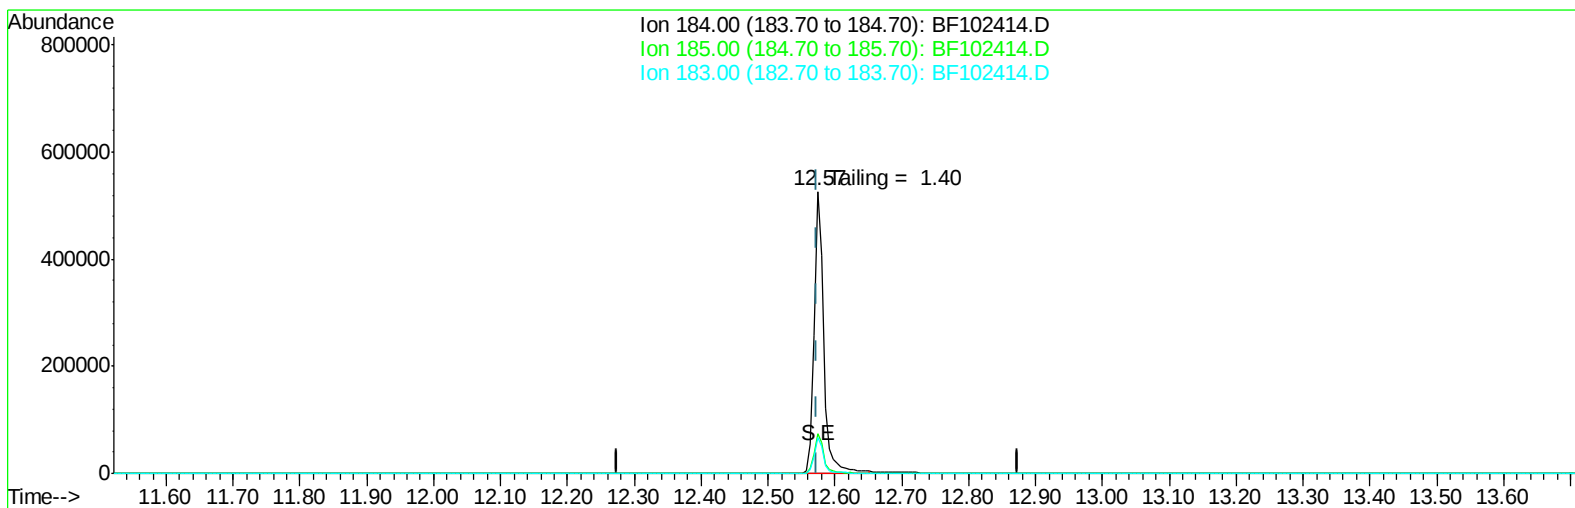

TIC: BF102414.D

(76) Benzidine



12.574min (+0.000) 0.00ng

response 542525

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.90
183.00	11.60	12.57
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF012518\
Data File : BF102414.D
Acq On : 25 Jan 2018 9:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 04:22:40 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 25 13:44:56 2018
Response via : Initial Calibration

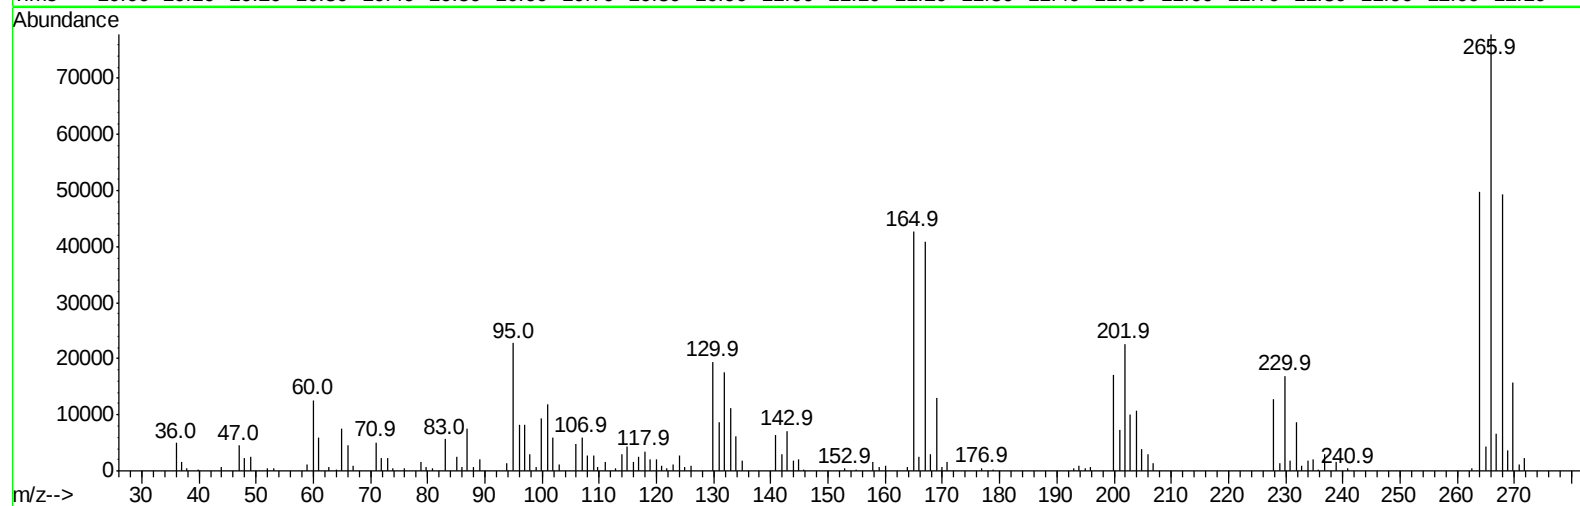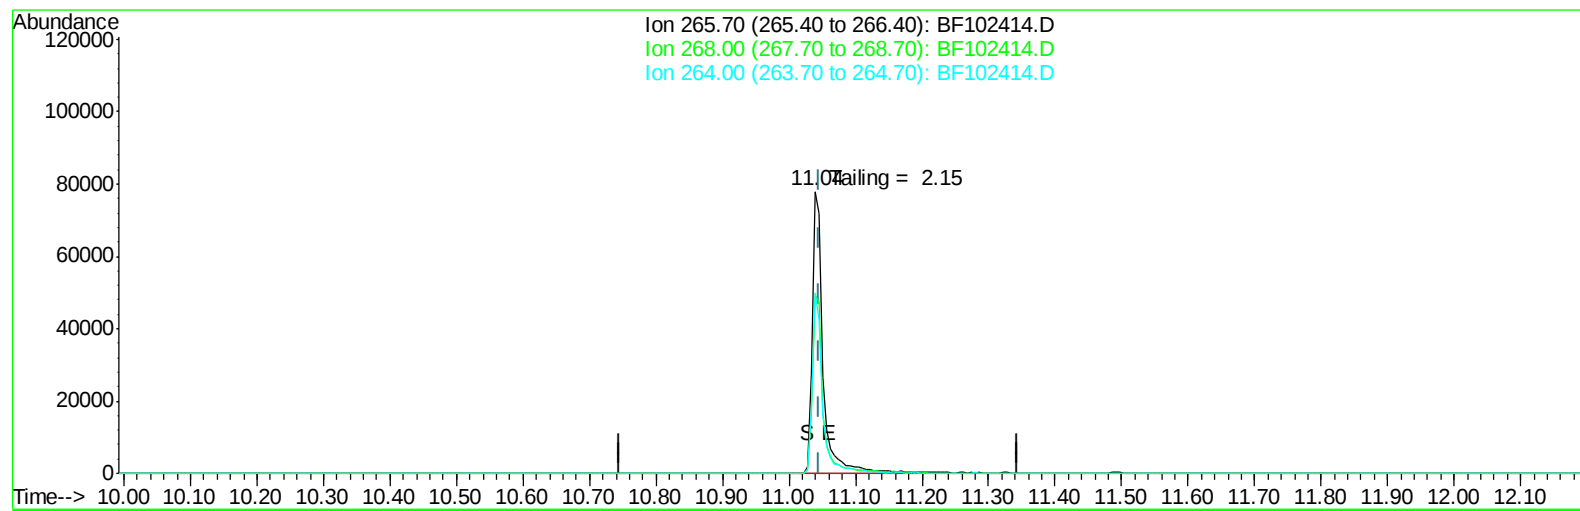

TIC: BF102414.D

(69) Pentachlorophenol (C)

11.039min (-0.006) 45216.56ng

response 89509

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.26
264.00	61.90	63.97
0.00	0.00	0.00