


Data Path : U:\HPCHEM1\BNA_F\Data\BF012518\
 Data File : BF102430.D
 Acq On : 25 Jan 2018 17:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 25 13:44:56 2018

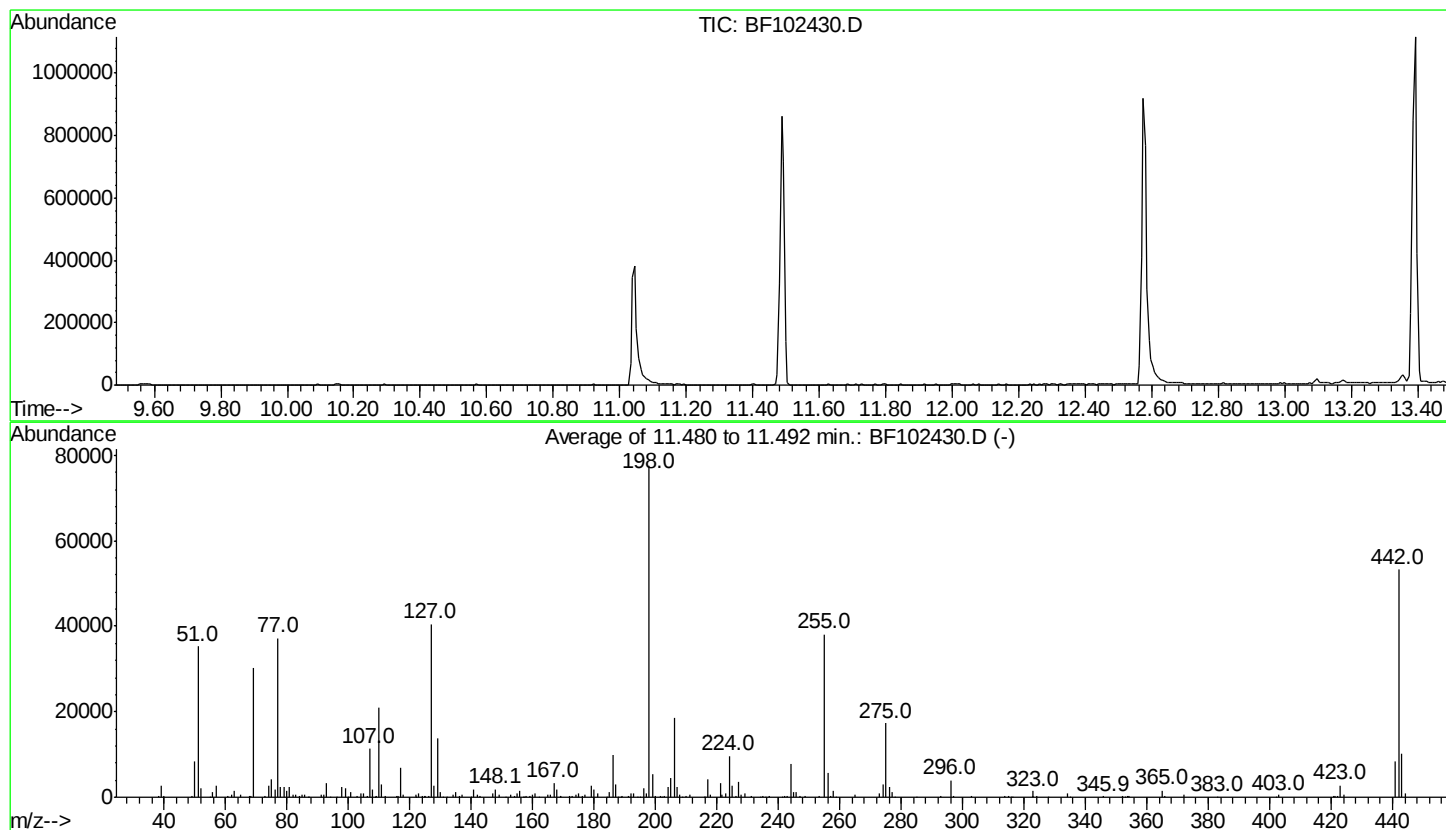

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	35266	PASS
68	69	0.00	2	1.0	300	PASS
69	198	0.00	100	38.9	30200	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	40496	PASS
197	198	0.00	2	1.1	869	PASS
198	198	100	100	100.0	77584	PASS
199	198	5	9	6.8	5302	PASS
275	198	10	60	22.4	17359	PASS
365	198	1	100	1.9	1509	PASS
441	443	0.01	100	84.6	8540	PASS
442	198	50	100	68.6	53196	PASS
443	442	15	24	19.0	10091	PASS