


Data Path : U:\HPCHEM1\BNA_F\Data\BF012518\
Data File : BF102456.D
Acq On : 26 Jan 2018 6:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 25 13:44:56 2018

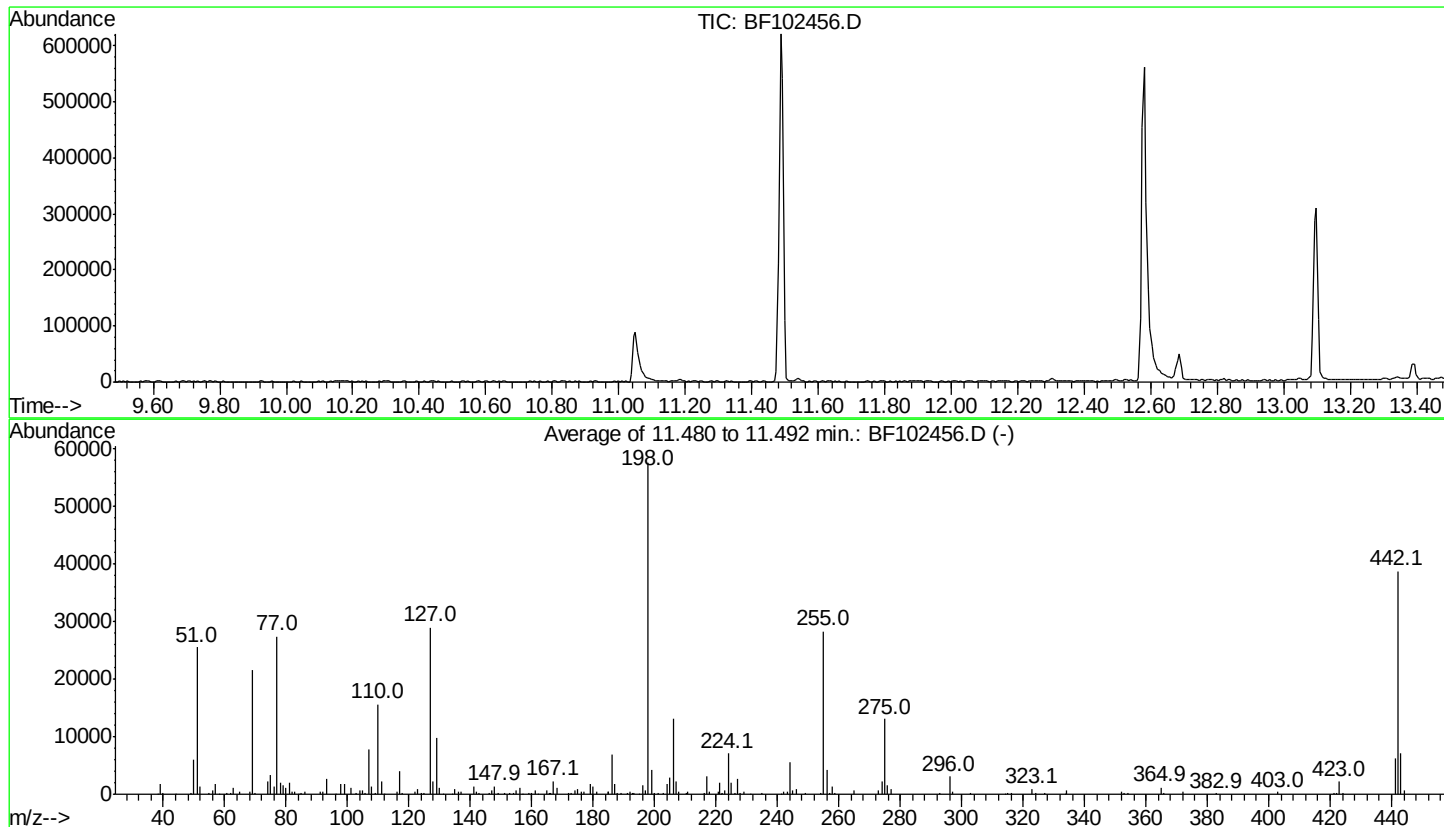

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	25490	PASS
68	69	0.00	2	2.0	435	PASS
69	198	0.00	100	37.5	21637	PASS
70	69	0.00	2	0.6	137	PASS
127	198	10	80	50.3	29000	PASS
197	198	0.00	2	1.2	711	PASS
198	198	100	100	100.0	57637	PASS
199	198	5	9	7.3	4204	PASS
275	198	10	60	22.6	13027	PASS
365	198	1	100	2.1	1219	PASS
441	443	0.01	100	85.3	6173	PASS
442	198	50	100	67.3	38779	PASS
443	442	15	24	18.7	7233	PASS