
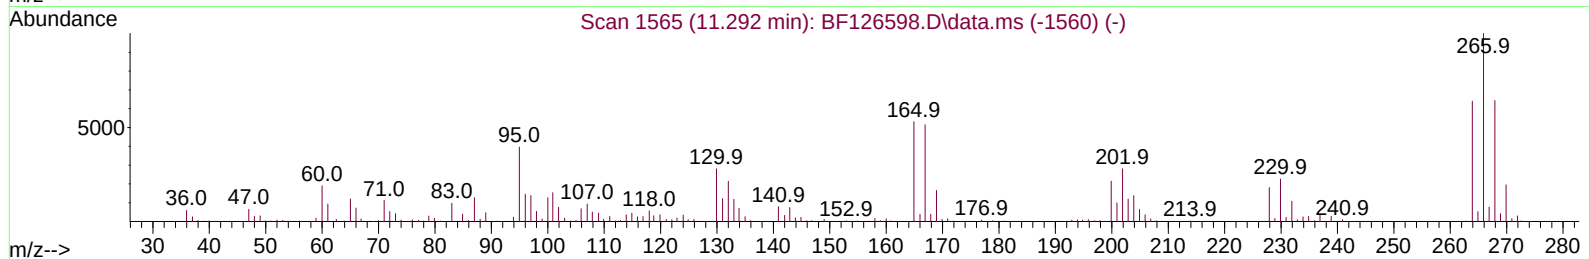
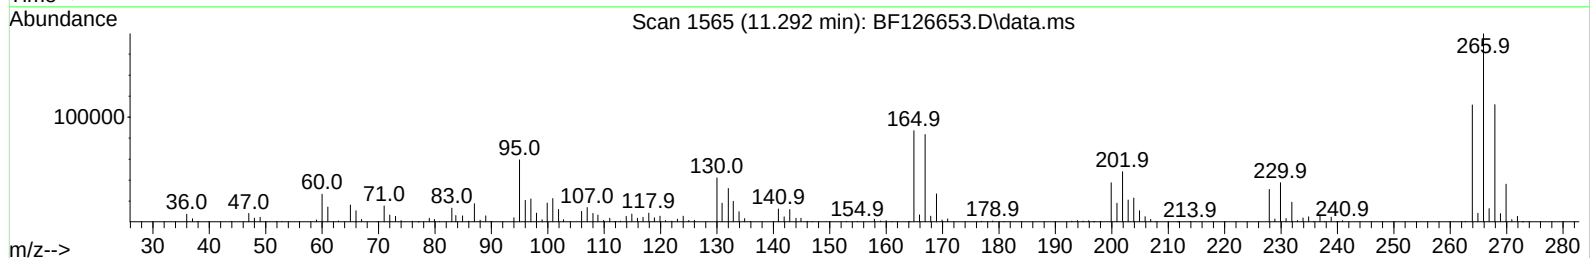


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012522\
Data File : BF126653.D
Acq On : 25 Jan 2022 09:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 04:46:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 19 07:04:14 2022
Response via : Initial Calibration

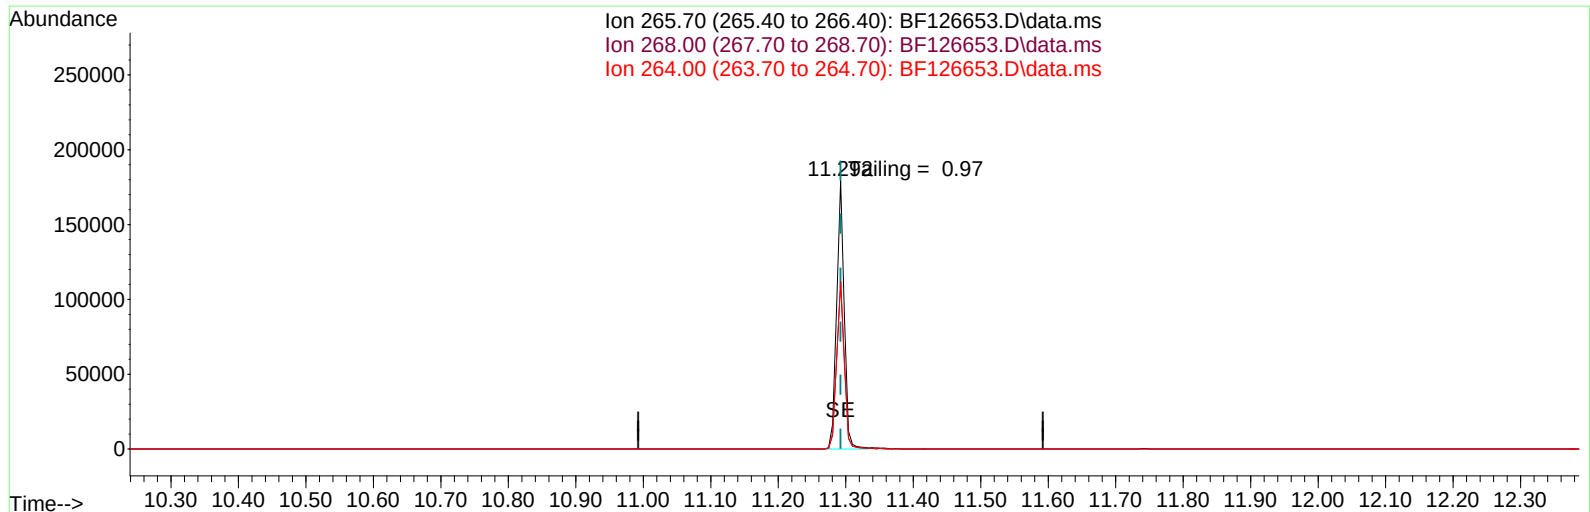

TIC: BF126653.D\data.ms

(70) Pentachlorophenol (C)




11.292min (+ 0.000) 33510.88 ng

response 142570

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	62.38
264.00	63.00	62.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012522\
Data File : BF126653.D
Acq On : 25 Jan 2022 09:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 04:46:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 19 07:04:14 2022
Response via : Initial Calibration

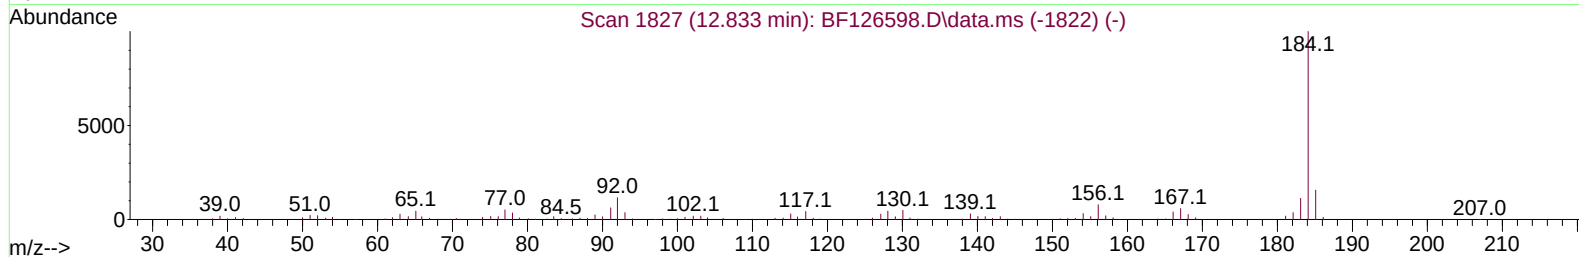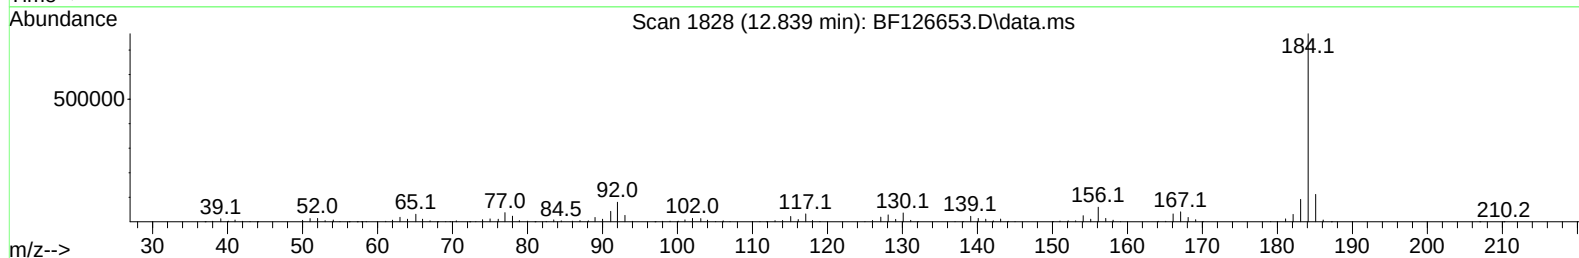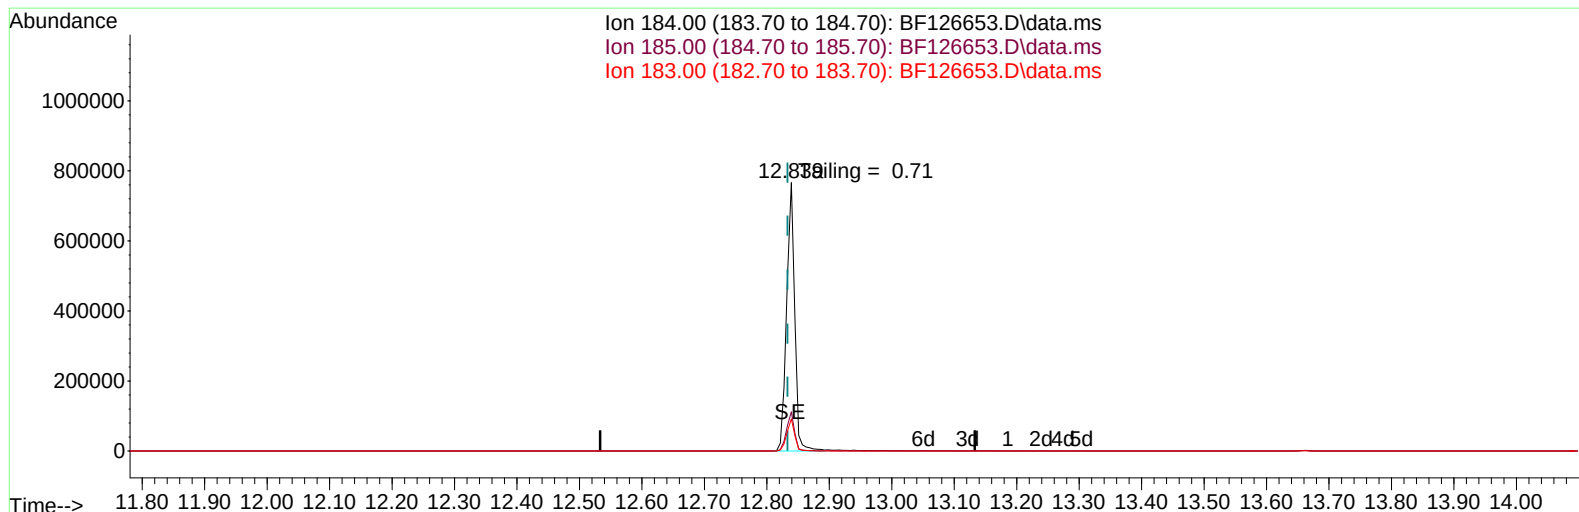

TIC: BF126653.D\data.ms

(77) Benzidine

12.839min (+ 0.006) 73759.59 ng m

response 704832

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.61
183.00	10.20	11.98
0.00	0.00	0.00