

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012522\
 Data File : BF126655.D
 Acq On : 25 Jan 2022 10:38
 Operator : CG/JU
 Sample : PB142212BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142212BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.357	36	46	51	rBV	132819	180821	3.19%	0.563%
2	5.593	590	596	599	rBV	4036064	4178558	73.79%	13.018%
3	6.581	757	764	767	rBV	3885115	4300509	75.94%	13.398%
4	6.963	825	829	832	rBV	1023163	812294	14.34%	2.531%
5	7.528	919	925	928	rBV	2671450	2894510	51.12%	9.018%
6	8.245	1042	1047	1050	rBV	1219971	1099001	19.41%	3.424%
7	9.322	1224	1230	1233	rBV	4404616	4716644	83.29%	14.694%
8	10.004	1341	1346	1350	rBV	1451426	1275760	22.53%	3.975%
9	10.798	1475	1481	1484	rBV	3376713	3144868	55.54%	9.798%
10	11.498	1596	1600	1603	rBV	1625679	1339281	23.65%	4.172%
11	13.092	1866	1871	1874	rBV	5638384	5662724	100.00%	17.642%
12	14.145	2046	2050	2058	rBV	1444196	1258795	22.23%	3.922%
13	15.674	2303	2310	2322	rVB	839428	1104000	19.50%	3.439%
14	16.168	2388	2394	2405	rVB2	44672	67257	1.19%	0.210%
15	16.715	2481	2487	2494	rBV2	34375	63565	1.12%	0.198%




Sum of corrected areas: 32098587

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012522\
Data File : BF126655.D
Acq On : 25 Jan 2022 10:38
Operator : CG/JU
Sample : PB142212BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142212BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

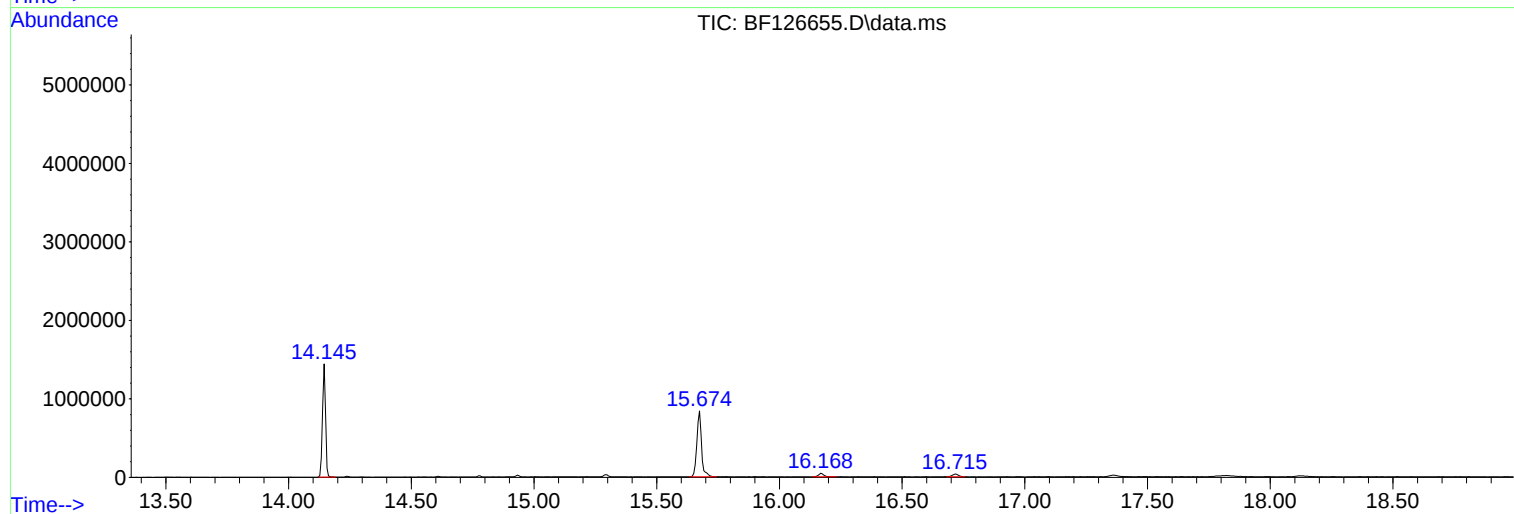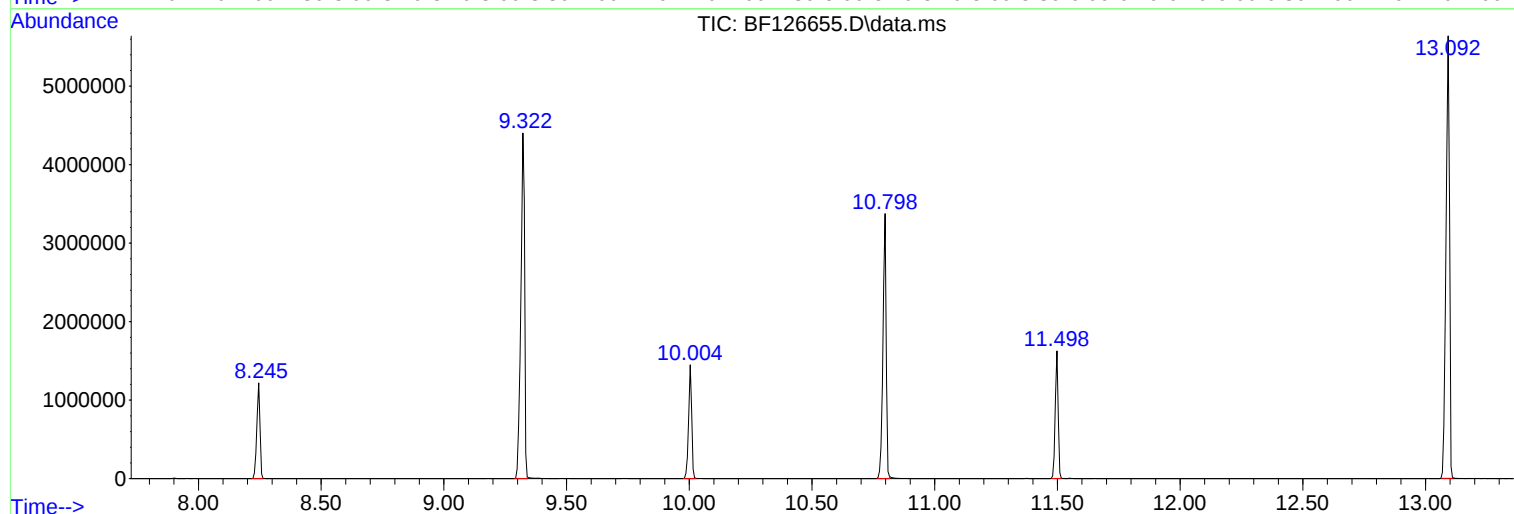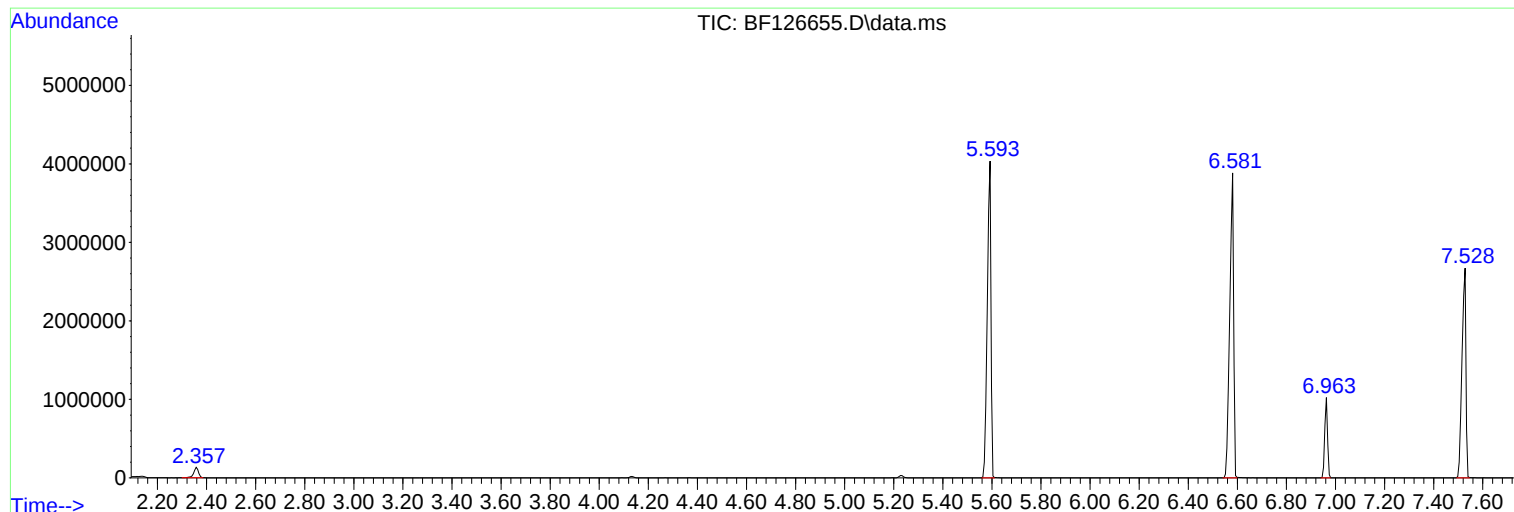

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012522\
Data File : BF126655.D
Acq On : 25 Jan 2022 10:38
Operator : CG/JU
Sample : PB142212BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142212BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.357	4.45 ng	180821	1,4-Dichlorobenzene-d4	6.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

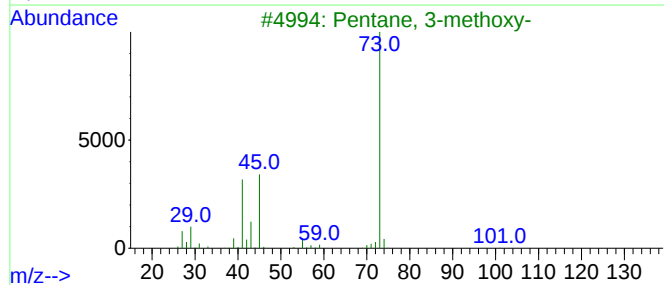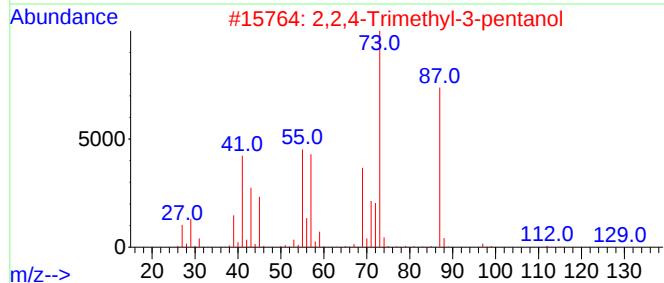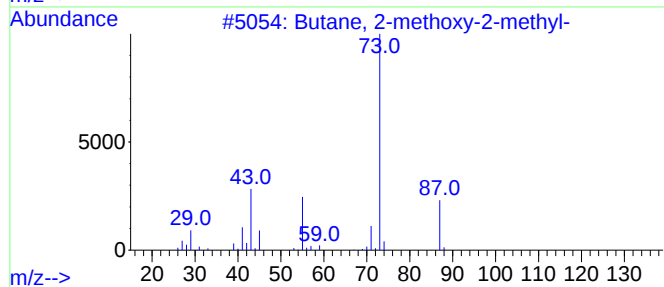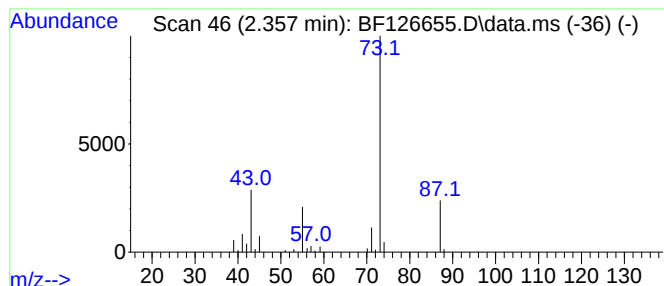

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012522\
Data File : BF126655.D
Acq On : 25 Jan 2022 10:38
Operator : CG/JU
Sample : PB142212BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142212BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.357	4.5	ng	180821	1	6.963	812294	20.0