
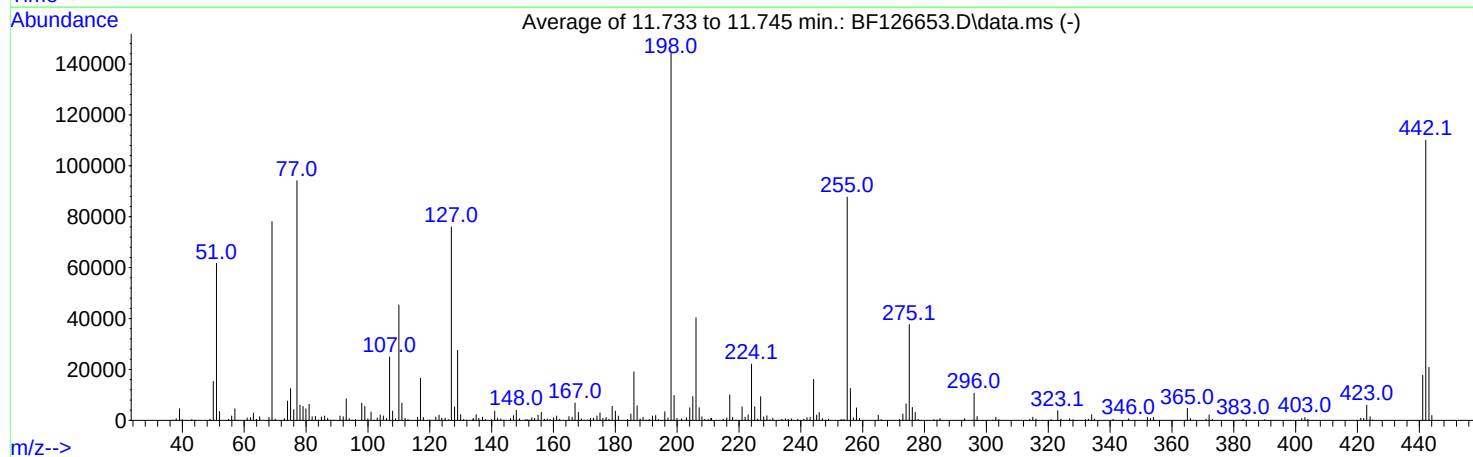


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012522\
 Data File : BF126653.D
 Acq On : 25 Jan 2022 09:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 19 07:04:14 2022

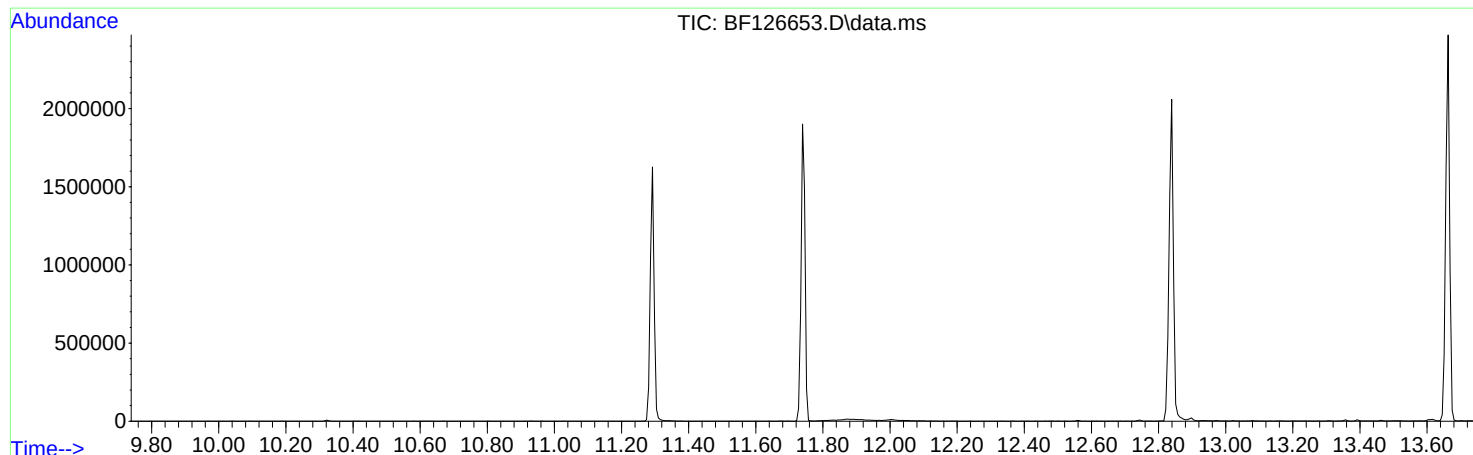


AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	61656	PASS
68	69	0.00	2	1.5	1192	PASS
69	198	0.00	100	54.1	78152	PASS
70	69	0.00	2	0.7	521	PASS
127	198	10	80	52.6	76000	PASS
197	198	0.00	2	0.7	966	PASS
198	198	100	100	100.0	144507	PASS
199	198	5	9	6.8	9780	PASS
275	198	10	60	26.1	37659	PASS
365	198	1	100	3.2	4696	PASS
441	198	0.01	100	12.3	17724	PASS
442	442	50	100	100.0	110043	PASS
443	442	15	24	19.0	20861	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012522\  
Data File : BF126653.D  
Acq On    : 25 Jan 2022  09:39  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 26 04:46:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 19 07:04:14 2022
Response via : Initial Calibration

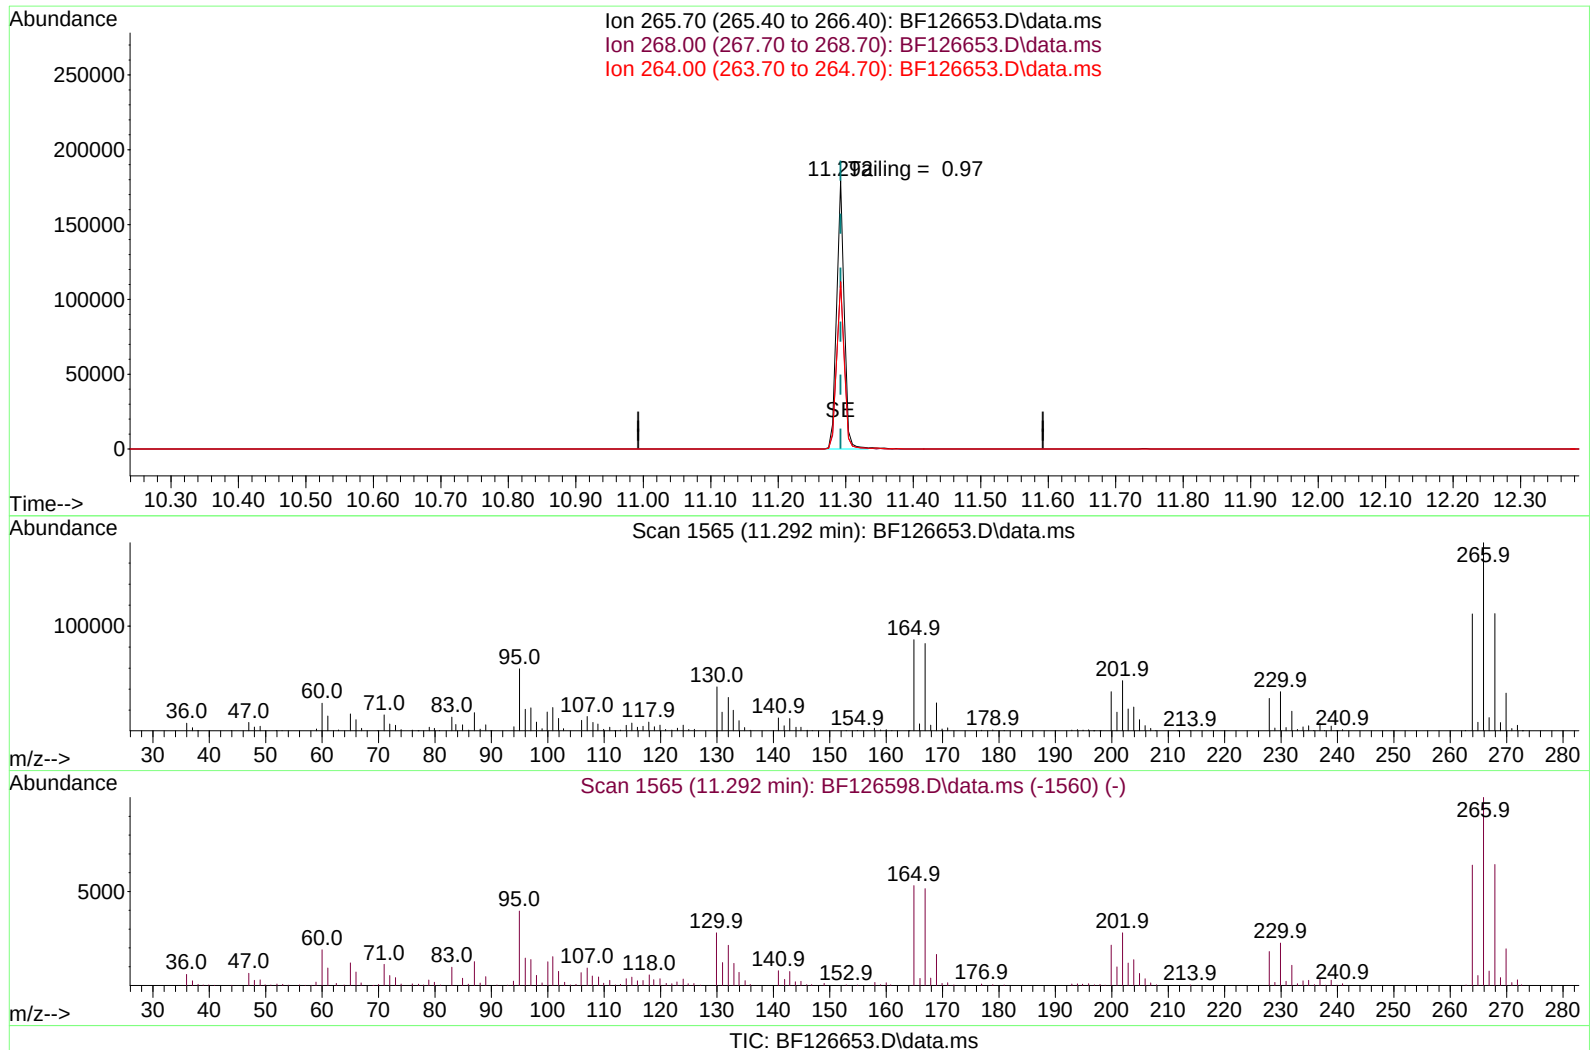

(70) Pentachlorophenol (C)

11.292min (+ 0.000) 33510.88 ng




response **142570**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	62.38
264.00	63.00	62.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012522\
Data File : BF126653.D
Acq On : 25 Jan 2022 09:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 26 04:46:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 19 07:04:14 2022
Response via : Initial Calibration

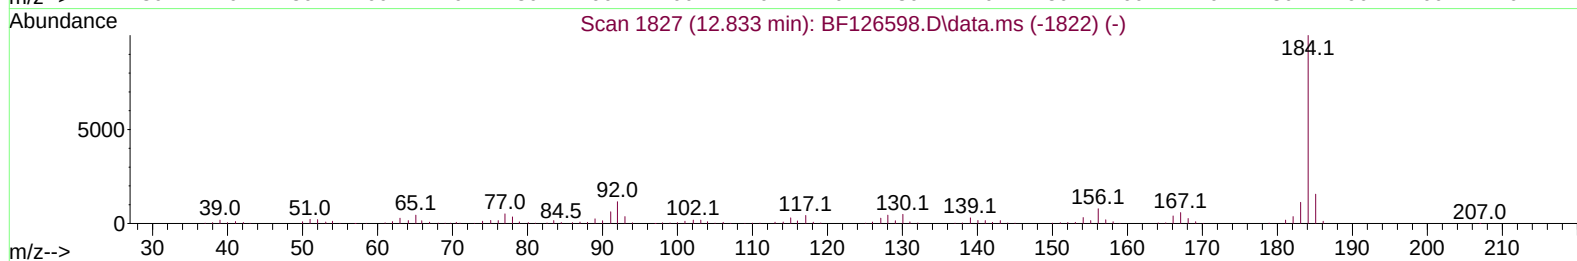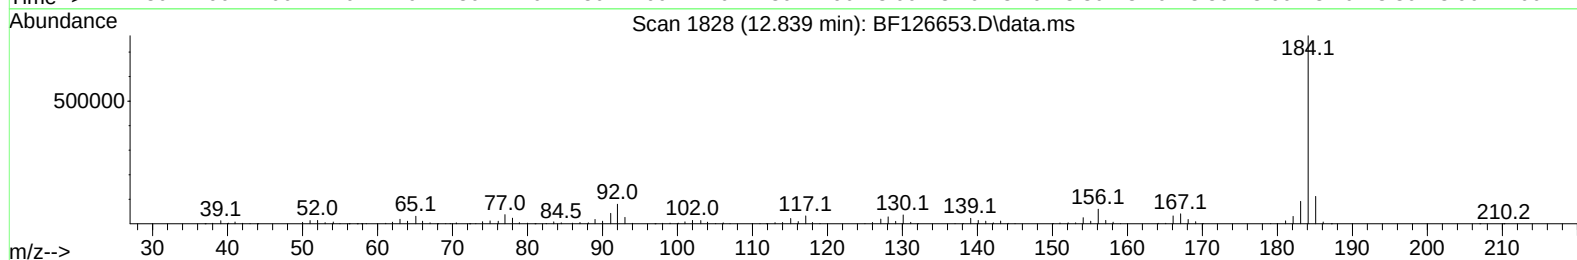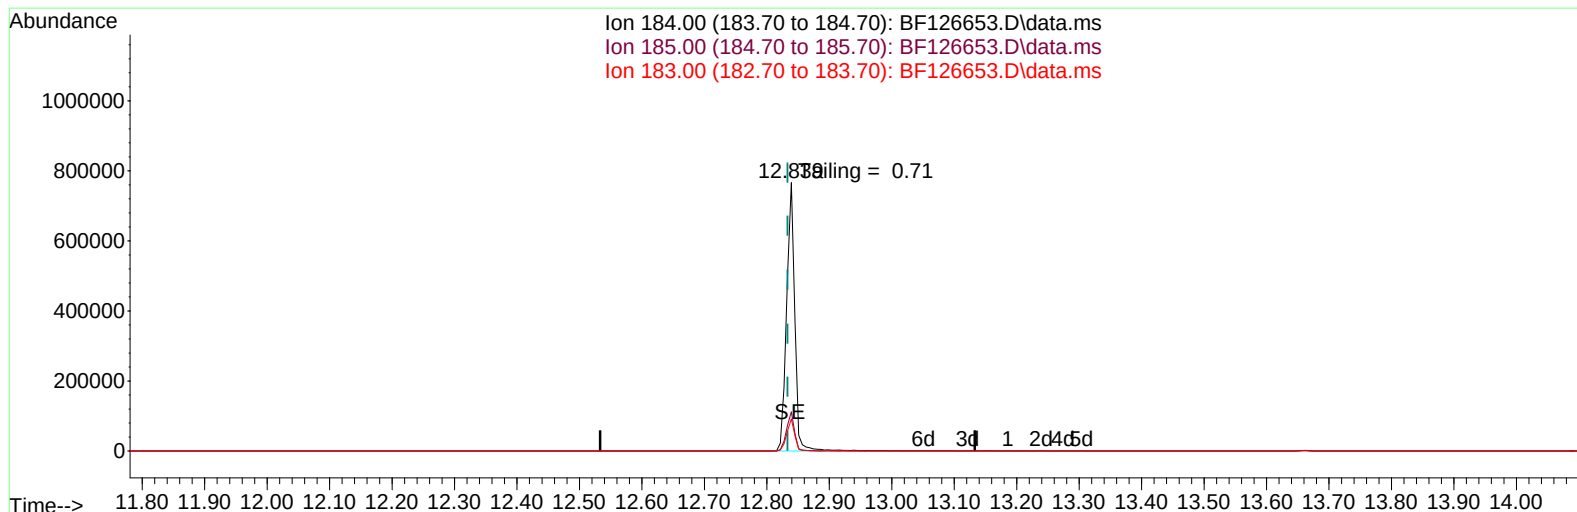

TIC: BF126653.D\data.ms

(77) Benzidine

12.839min (+ 0.006) 73759.59 ng m

response 704832

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.61
183.00	10.20	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/25/2022	BNA_F	<u>BF126653.D</u>
Compound Name	Response	Retention Time
DDT	363848	13.663
DDD	3026	13.392
DDE	255	13.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3281	367129	0.89

Instrument :
BNA_F
ClientSampleId :
DFTPP