
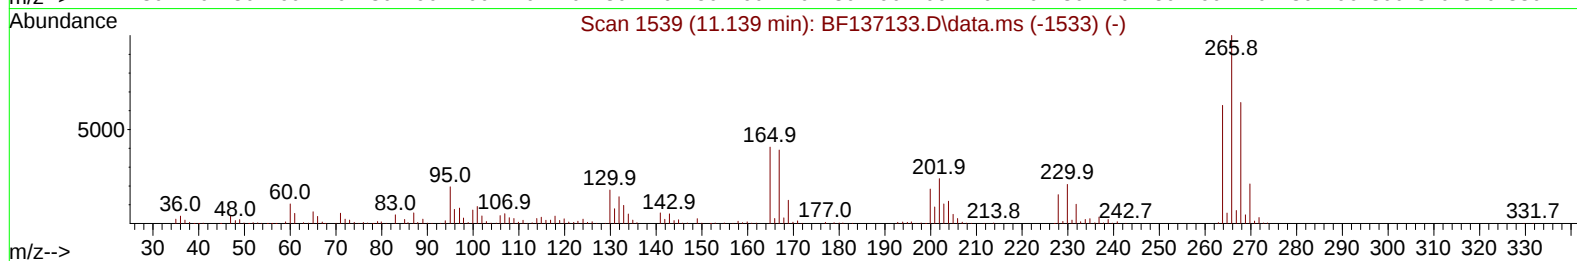
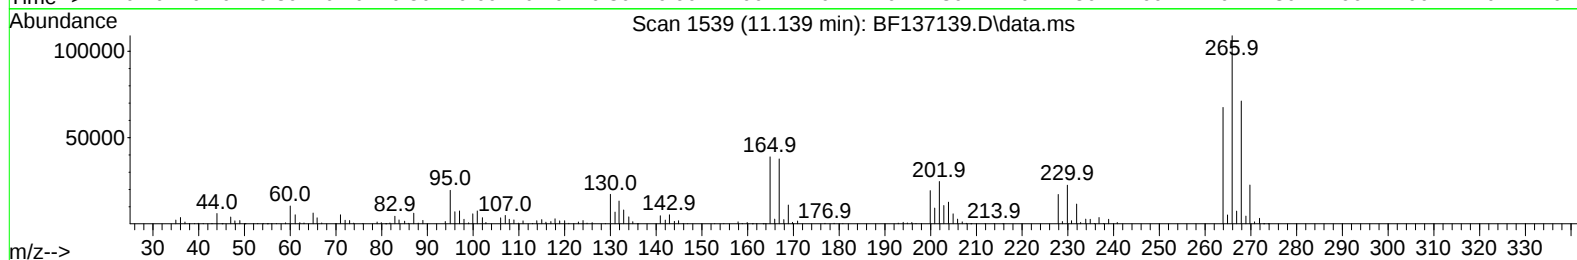


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012524\
Data File : BF137139.D
Acq On : 25 Jan 2024 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 12:00:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 03:53:23 2024
Response via : Initial Calibration

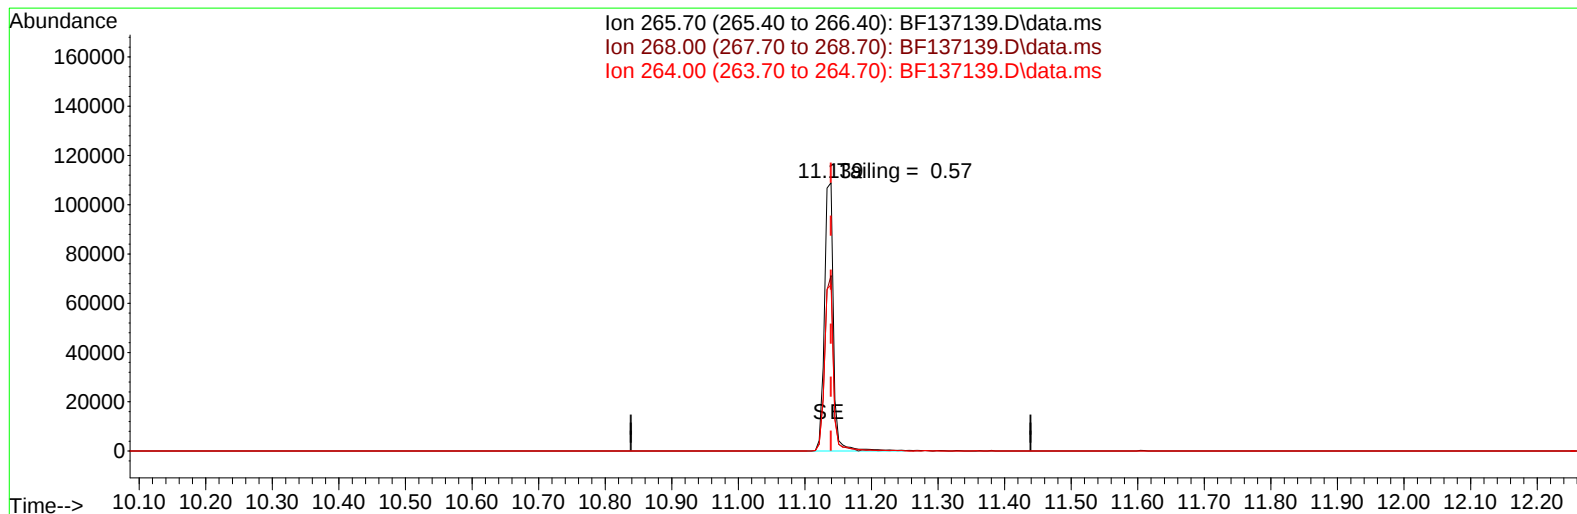

TIC: BF137139.D\data.ms

(70) Pentachlorophenol (C)




11.139min (+ 0.000) 26977.63 ng

response 103298

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	65.32
264.00	62.80	61.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012524\
Data File : BF137139.D
Acq On : 25 Jan 2024 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 12:00:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 24 03:53:23 2024
Response via : Initial Calibration

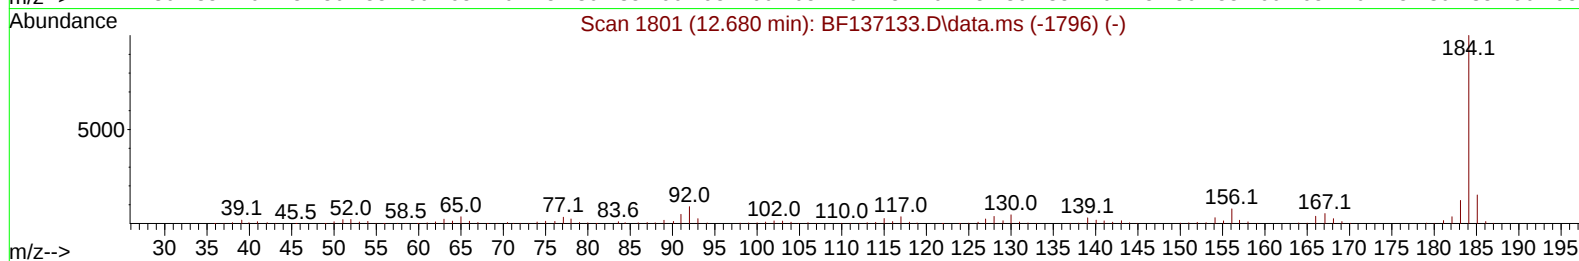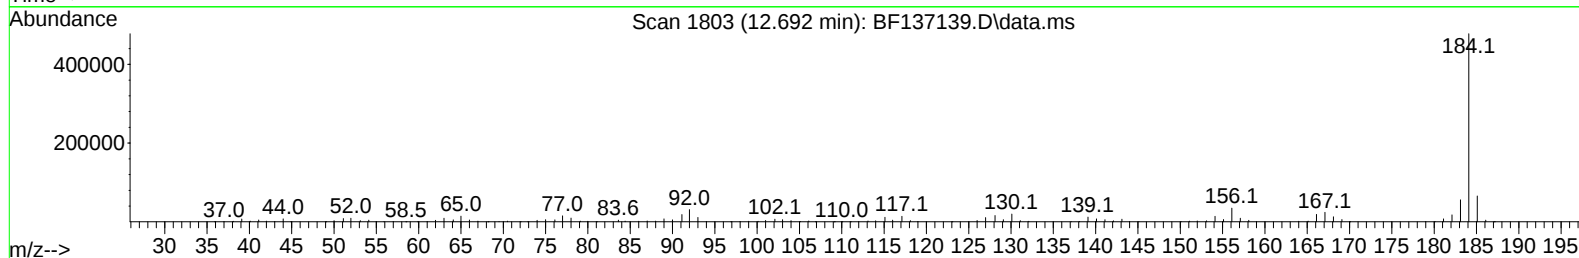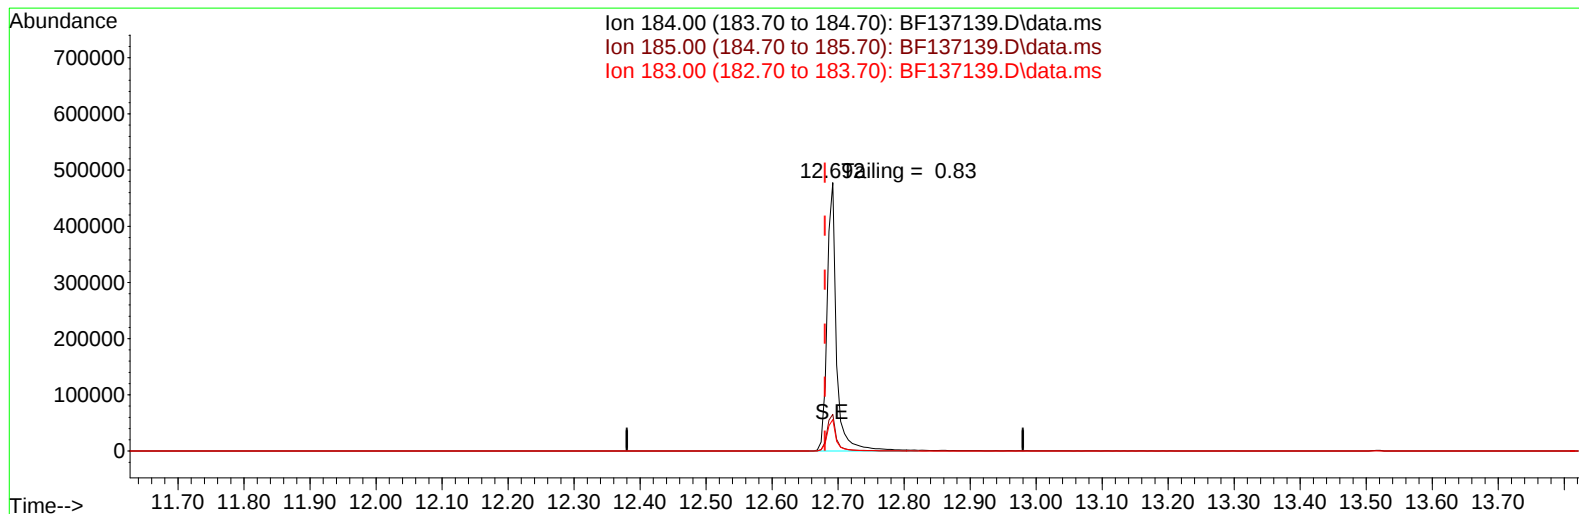

TIC: BF137139.D\data.ms

(77) Benzidine

12.692min (+ 0.012) 0.00 ng m

response 473037

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.70
183.00	12.30	11.68
0.00	0.00	0.00