


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012524\
Data File : BF137139.D
Acq On : 25 Jan 2024 10:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 25 23:14:32 2024

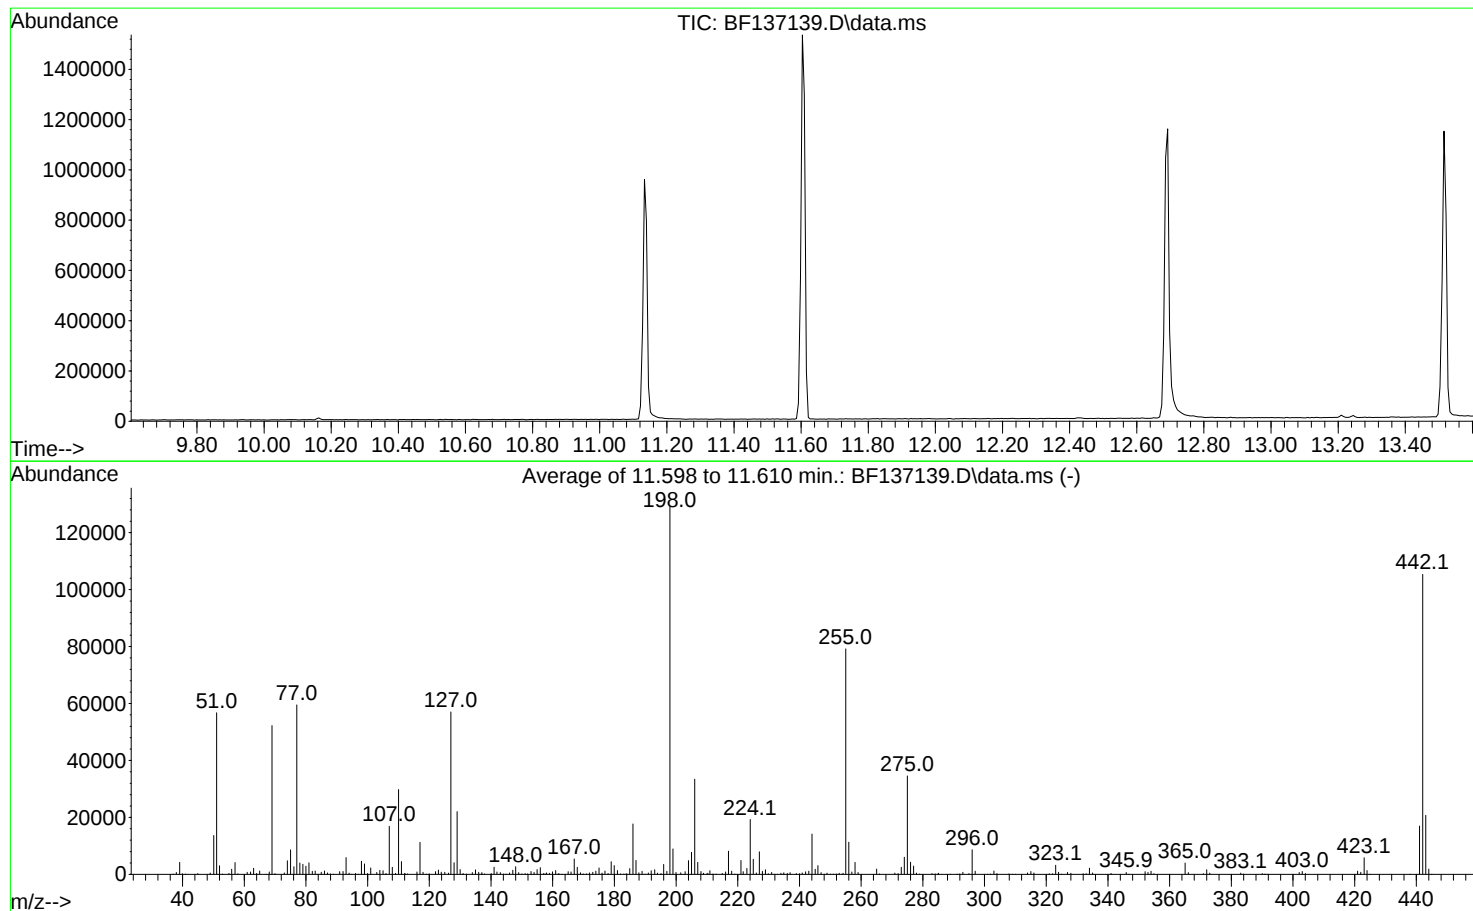




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	56757	PASS
68	69	0.00	2	1.6	833	PASS
69	198	0.00	100	40.4	52240	PASS
70	69	0.00	2	0.4	233	PASS
127	198	10	80	44.1	57032	PASS
197	198	0.00	2	0.8	1069	PASS
198	198	100	100	100.0	129184	PASS
199	198	5	9	6.9	8946	PASS
275	198	10	60	26.8	34570	PASS
365	198	1	100	3.1	4010	PASS
441	198	0.01	100	13.2	16998	PASS
442	442	50	100	100.0	105389	PASS
443	442	15	24	19.7	20721	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012524\
 Data File : BF137139.D
 Acq On : 25 Jan 2024 10:28
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 25 12:00:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF012524.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 24 03:53:23 2024
 Response via : Initial Calibration

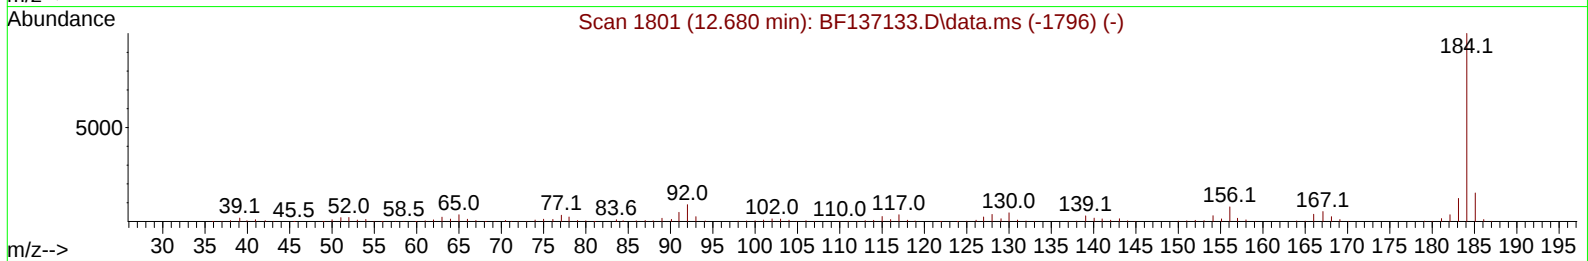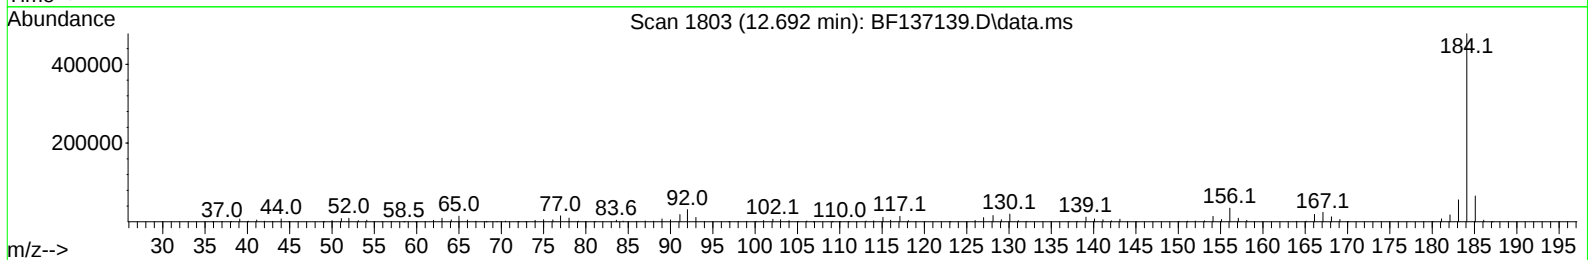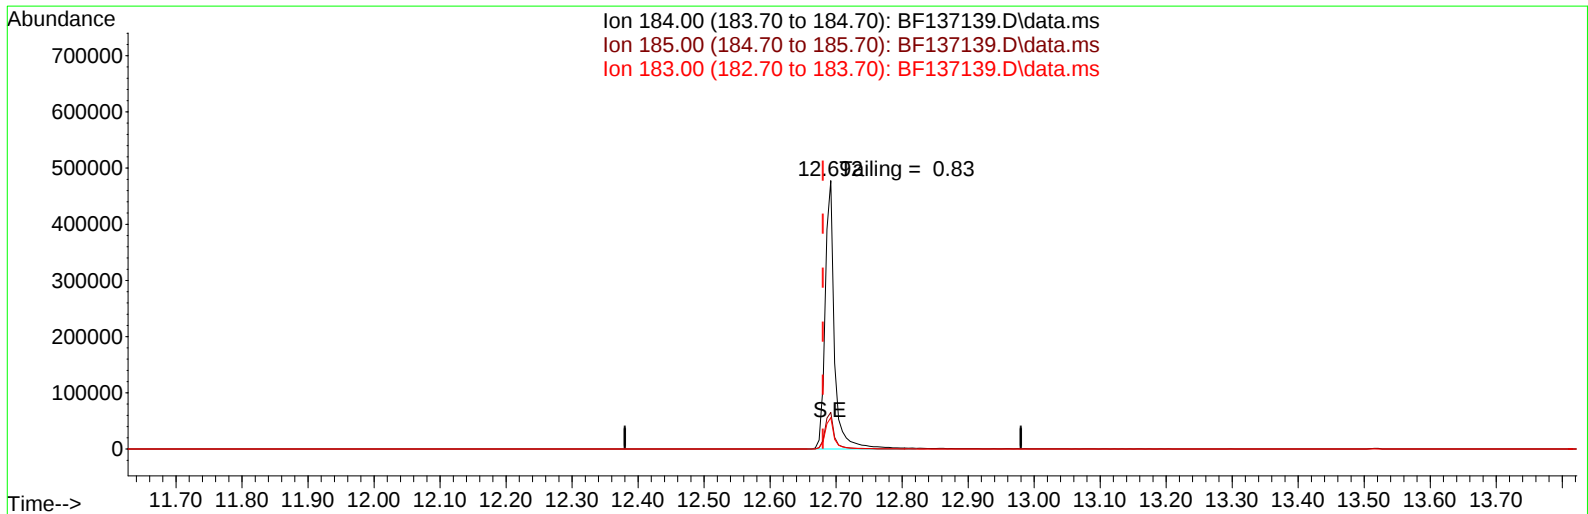

TIC: BF137139.D\data.ms

(77) Benzidine

12.692min (+ 0.012) 0.00 ng m

response 473037

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.70
183.00	12.30	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/25/2024	BNA_F	<u>BF137139.D</u>
Compound Name	Response	Retention Time
DDT	131485	13.515
DDD	2271	13.21
DDE	55	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2326	133811	1.74

Instrument :
BNA_F
ClientSampleId :
DFTPP