

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012615\
 Data File : BF077059.D
 Acq On : 26 Jan 2015 18:39
 Operator : TP/IZ
 Sample : PB81509BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB81509BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.327	19	21	26	rBV	14794	27300	3.22%	0.469%
2	1.407	26	28	41	rVB	23840	54555	6.44%	0.938%
3	3.841	239	241	256	rBV	29963	75304	8.89%	1.294%
4	4.790	321	324	336	rBV	293527	571343	67.48%	9.819%
5	7.167	529	532	537	rBV	356483	557476	65.85%	9.581%
6	7.259	537	540	546	rVB	341496	625886	73.93%	10.756%
7	7.762	581	584	591	rVB	77898	123671	14.61%	2.125%
8	8.082	609	612	620	rVB	300091	470432	55.56%	8.085%
9	9.065	695	698	708	rBV	239043	362021	42.76%	6.222%
10	10.676	836	839	842	rBV	108427	171594	20.27%	2.949%
11	13.328	1067	1071	1074	rBV	468273	729564	86.17%	12.538%
12	14.802	1196	1200	1204	rVB	114551	191051	22.57%	3.283%
13	16.517	1347	1350	1353	rBV	333638	430137	50.81%	7.392%
14	17.626	1445	1447	1450	rBV	144077	199226	23.53%	3.424%
15	19.877	1641	1644	1646	rBV	765490	846643	100.00%	14.550%
16	21.134	1752	1754	1757	rBV	173752	196764	23.24%	3.382%
17	22.769	1894	1897	1900	rBV	156559	185761	21.94%	3.192%




Sum of corrected areas: 5818728

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012615\
Data File : BF077059.D
Acq On : 26 Jan 2015 18:39
Operator : TP/IZ
Sample : PB81509BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81509BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

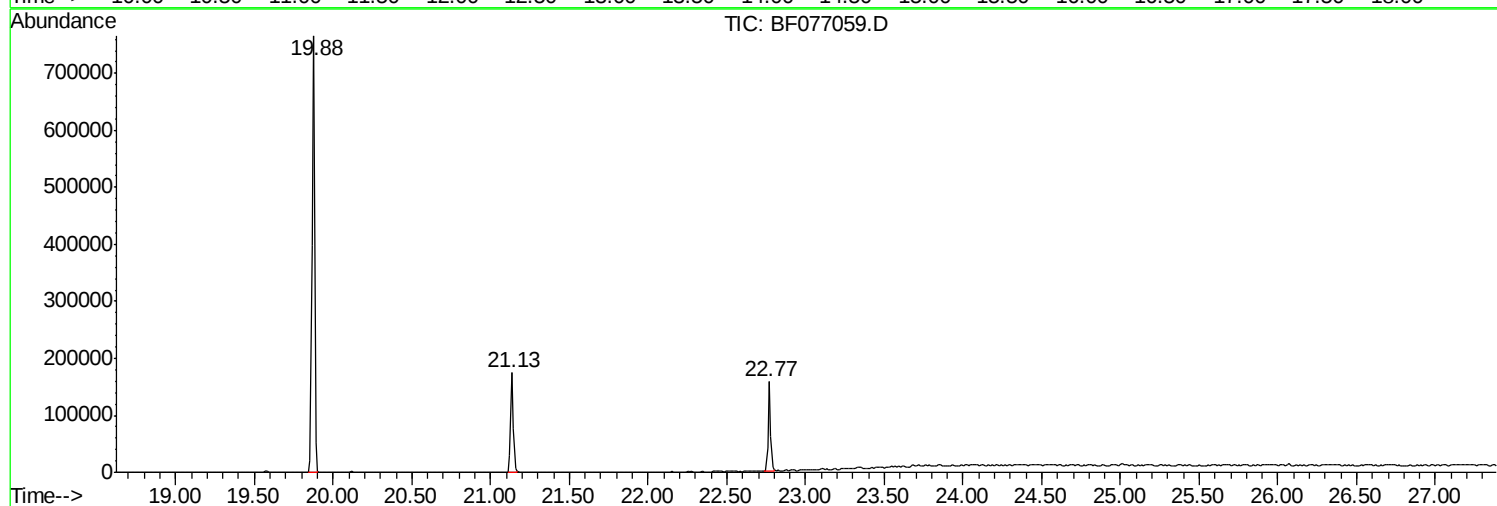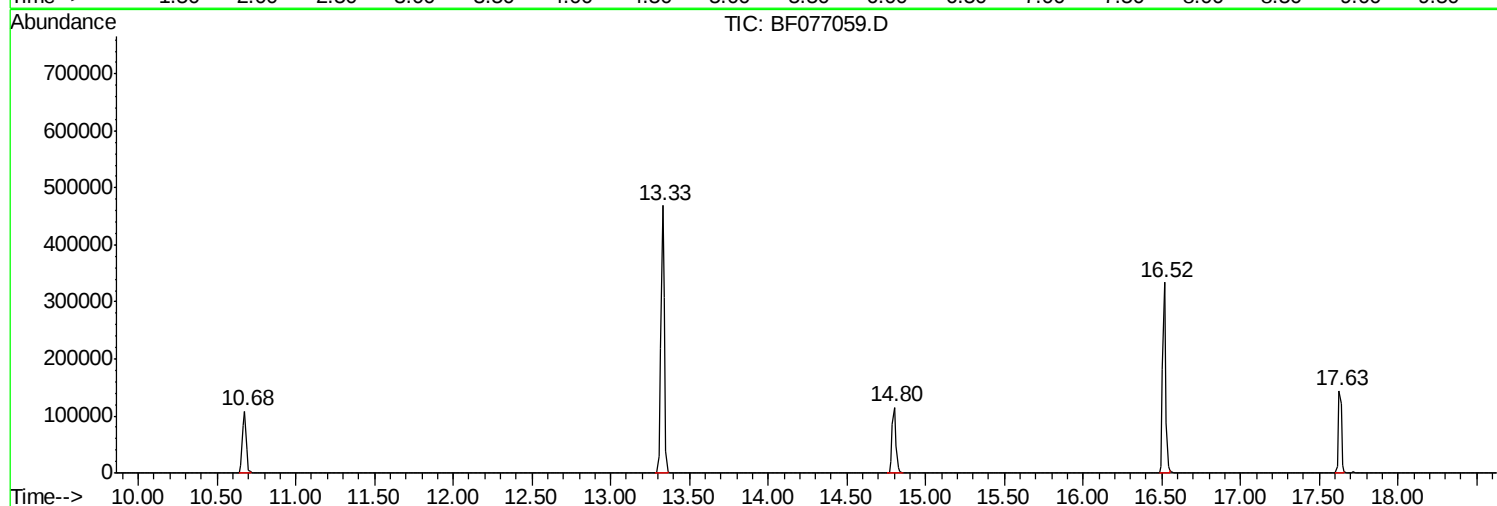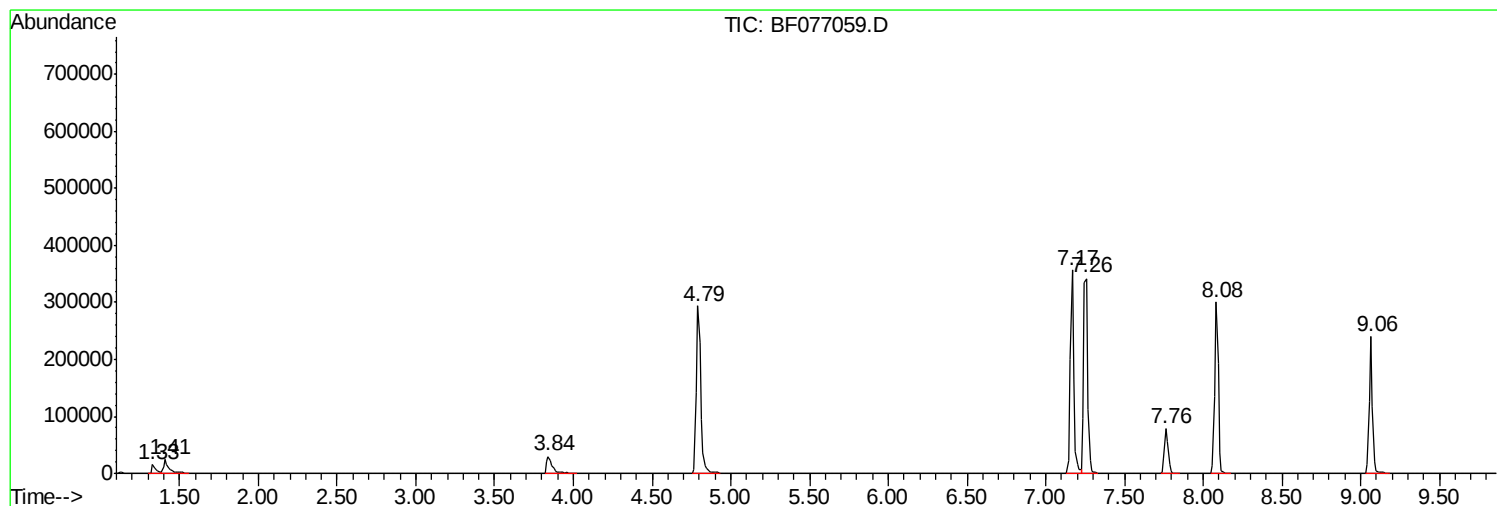

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012615\
Data File : BF077059.D
Acq On : 26 Jan 2015 18:39
Operator : TP/IZ
Sample : PB81509BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
PB81509BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown3.84 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.84	12.18 ng	75304	1,4-Dichlorobenzene-d4	7.76

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,8-Nonanediol, 8-methyl-	174	C10H22O2	054725-73-4	42
2		3-Octanol	130	C8H18O	000589-98-0	38
3		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	38
4		Guanidine	59	CH5N3	000113-00-8	9
5		5-Hexen-2-one	98	C6H10O	000109-49-9	9

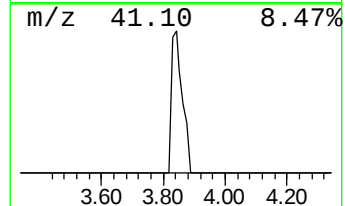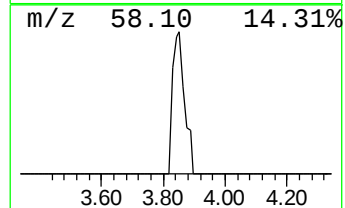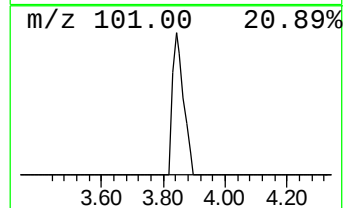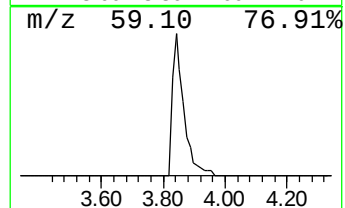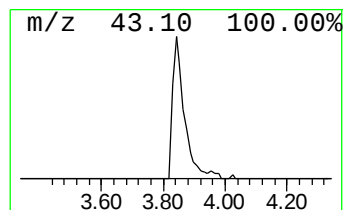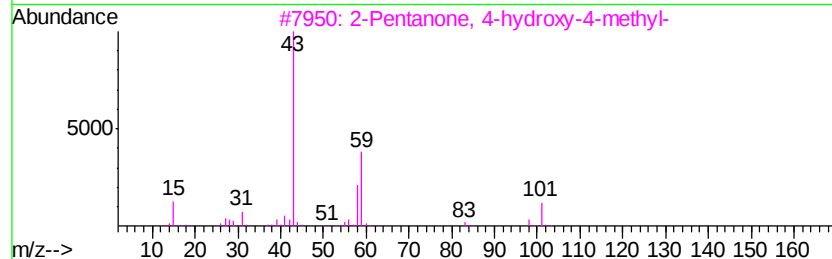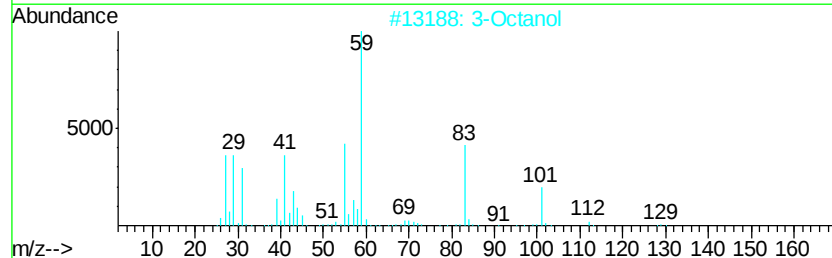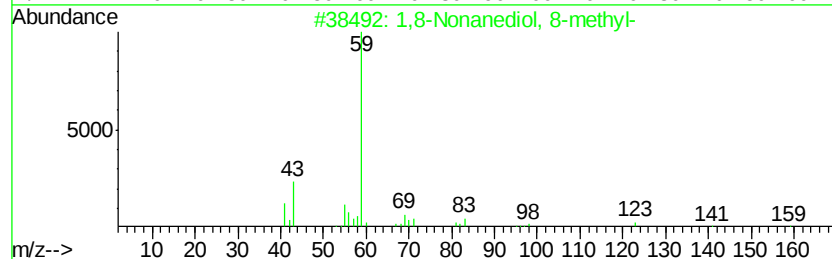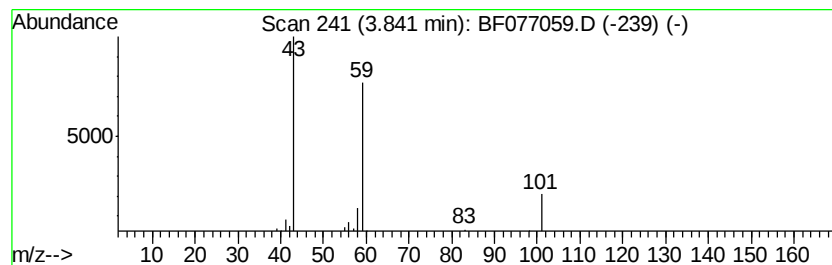

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012615\
Data File : BF077059.D
Acq On : 26 Jan 2015 18:39
Operator : TP/IZ
Sample : PB81509BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81509BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown7.26 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.26	101.22 ng	625886	1,4-Dichlorobenzene-d4	7.76

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	25
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

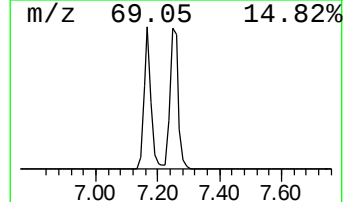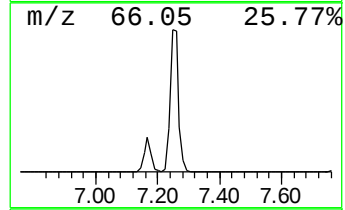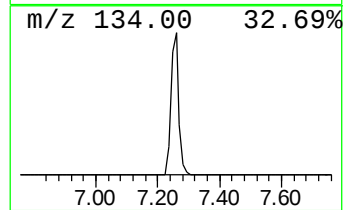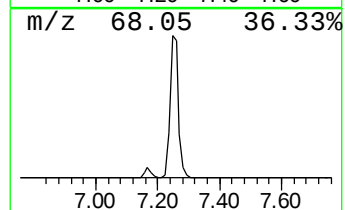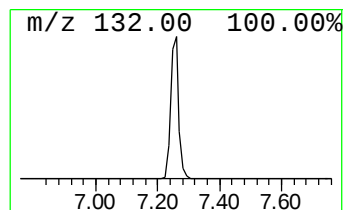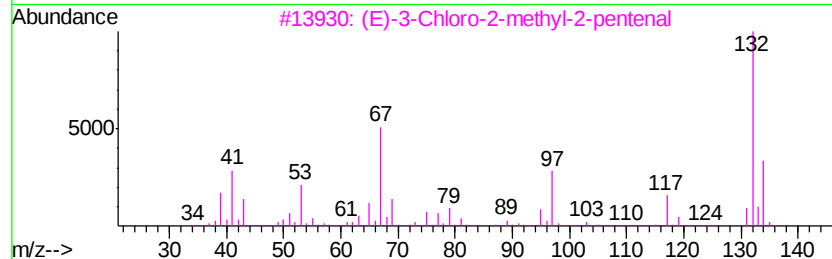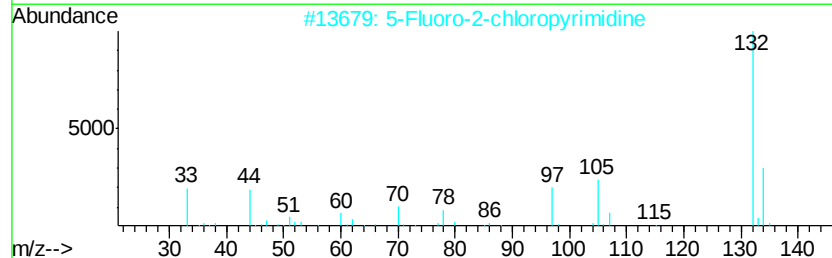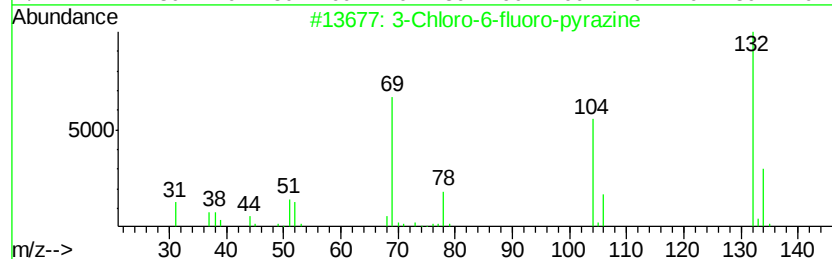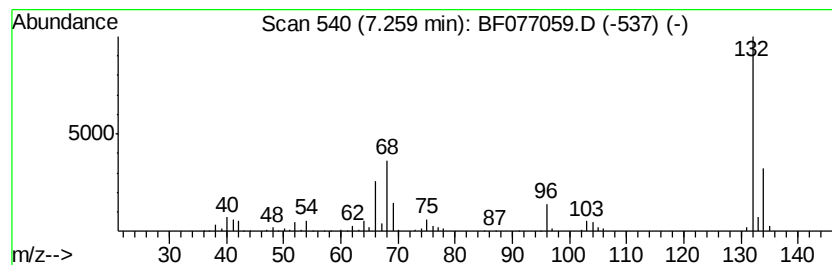

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012615\
Data File : BF077059.D
Acq On : 26 Jan 2015 18:39
Operator : TP/IZ
Sample : PB81509BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81509BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown3.84	3.84	12.2	ng	75304	1	7.76	123671	20.0
unknown7.26	7.26	101.2	ng	625886	1	7.76	123671	20.0