


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012615\
 Data File : BF077046.D
 Acq On : 26 Jan 2015 9:50
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 28 16:07:35 2015

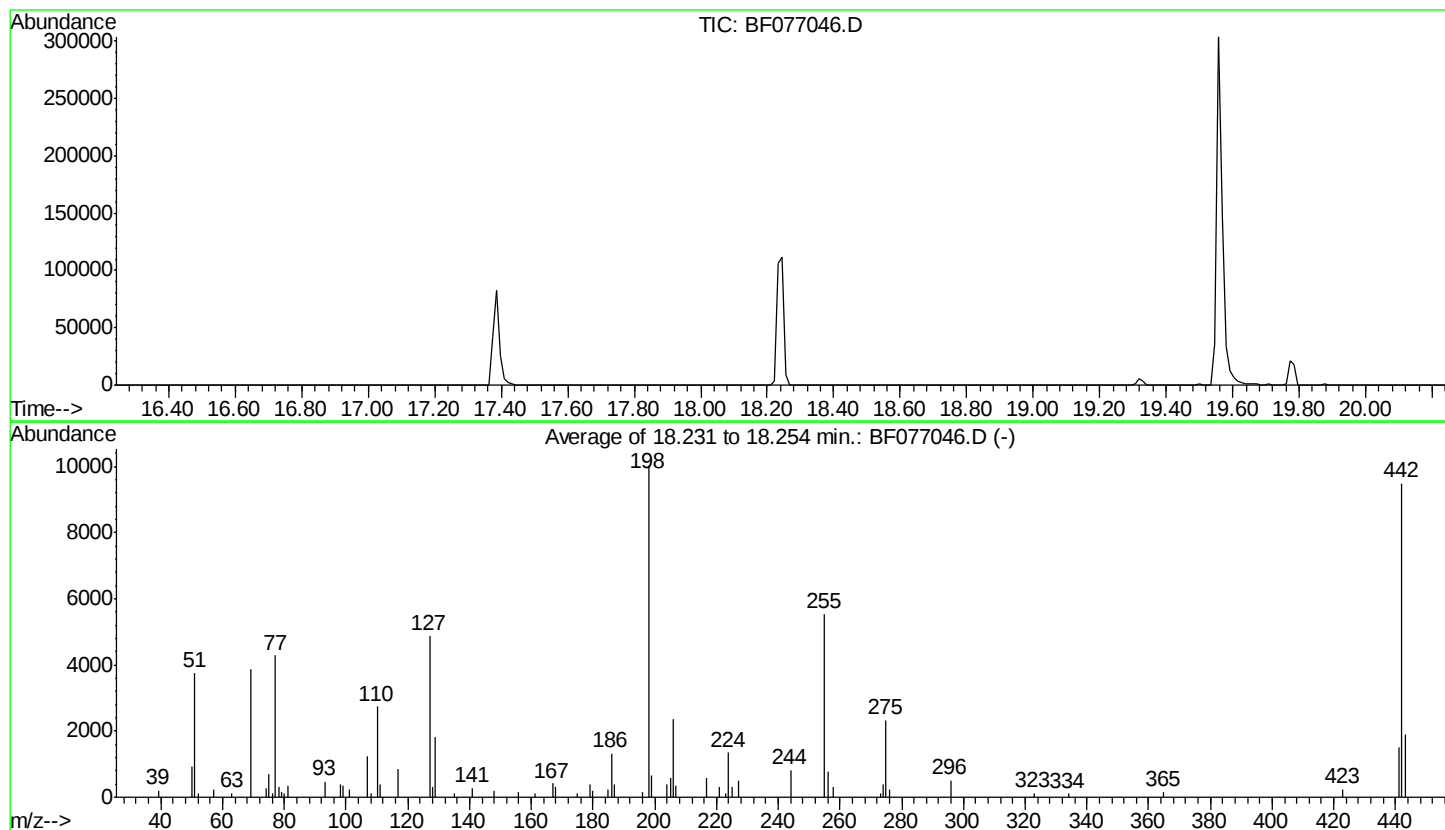

AutoFind: Scans 1500, 1501, 1502; Background Corrected with Scan 1496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	3773	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.5	3865	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	4883	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10031	PASS
199	198	5	9	6.6	661	PASS
275	198	10	60	23.2	2324	PASS
365	198	1	100	1.6	164	PASS
441	442	0.01	24	16.1	1529	PASS
442	198	50	100	94.6	9491	PASS
443	442	15	24	20.2	1916	PASS