


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF012615\  
Data File : BF077065.D  
Acq On : 26 Jan 2015 23:03  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF011415.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Jan 28 16:07:35 2015

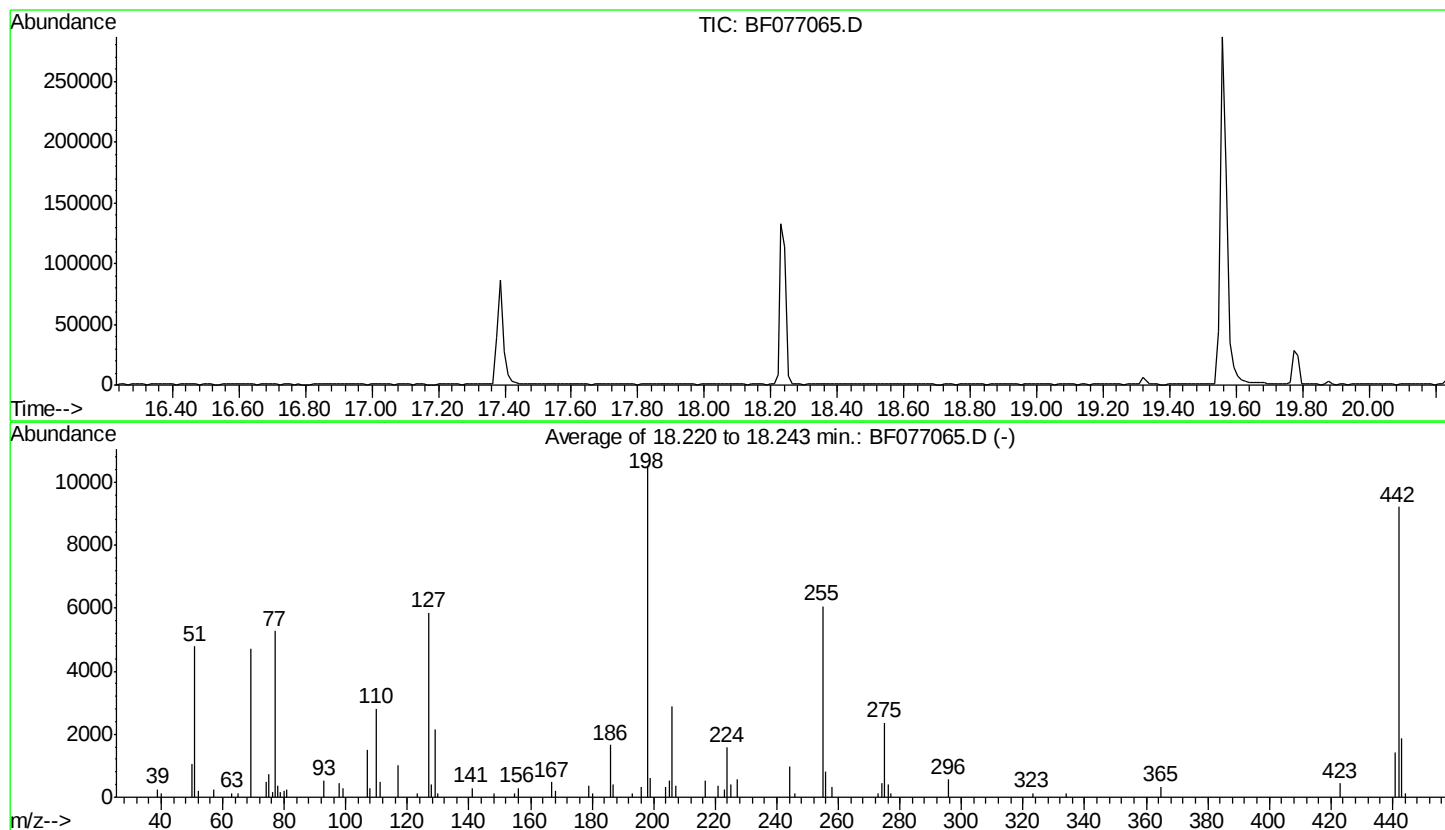

AutoFind: Scans 1499, 1500, 1501; Background Corrected with Scan 1496

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 45.5      | 4785    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 44.8      | 4712    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 55.7      | 5858    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 10517   | PASS             |
| 199         | 198          | 5            | 9            | 5.8       | 609     | PASS             |
| 275         | 198          | 10           | 60           | 22.5      | 2367    | PASS             |
| 365         | 198          | 1            | 100          | 3.2       | 339     | PASS             |
| 441         | 442          | 0.01         | 24           | 15.6      | 1441    | PASS             |
| 442         | 198          | 50           | 100          | 87.6      | 9213    | PASS             |
| 443         | 442          | 15           | 24           | 20.4      | 1882    | PASS             |