


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012615\
 Data File : BF077085.D
 Acq On : 27 Jan 2015 12:39
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF011415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 28 16:07:35 2015

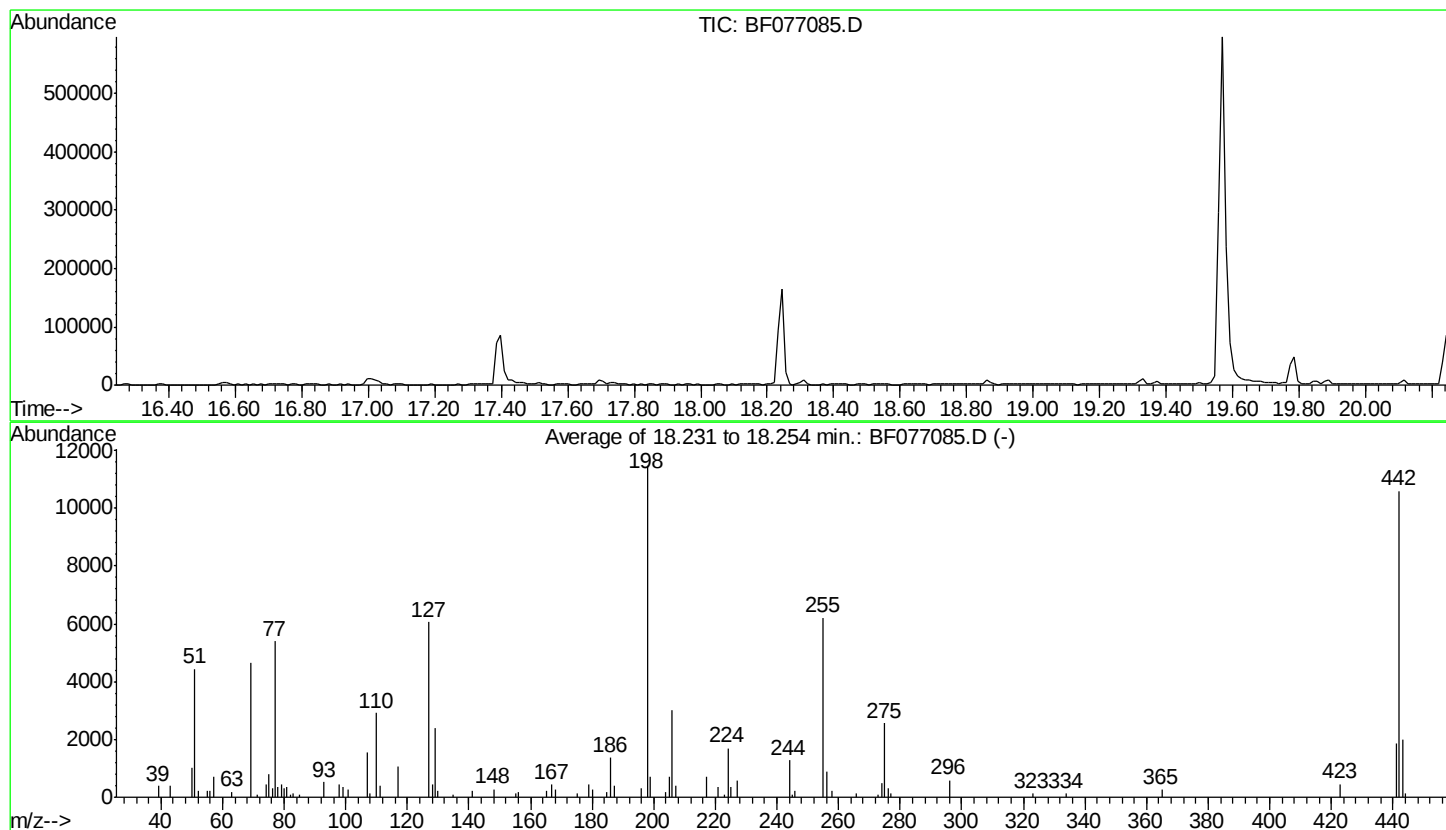

AutoFind: Scans 1500, 1501, 1502; Background Corrected with Scan 1496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	4435	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.4	4637	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.8	6060	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11472	PASS
199	198	5	9	6.4	731	PASS
275	198	10	60	22.2	2549	PASS
365	198	1	100	2.2	254	PASS
441	442	0.01	24	17.6	1864	PASS
442	198	50	100	92.3	10588	PASS
443	442	15	24	18.9	1996	PASS