
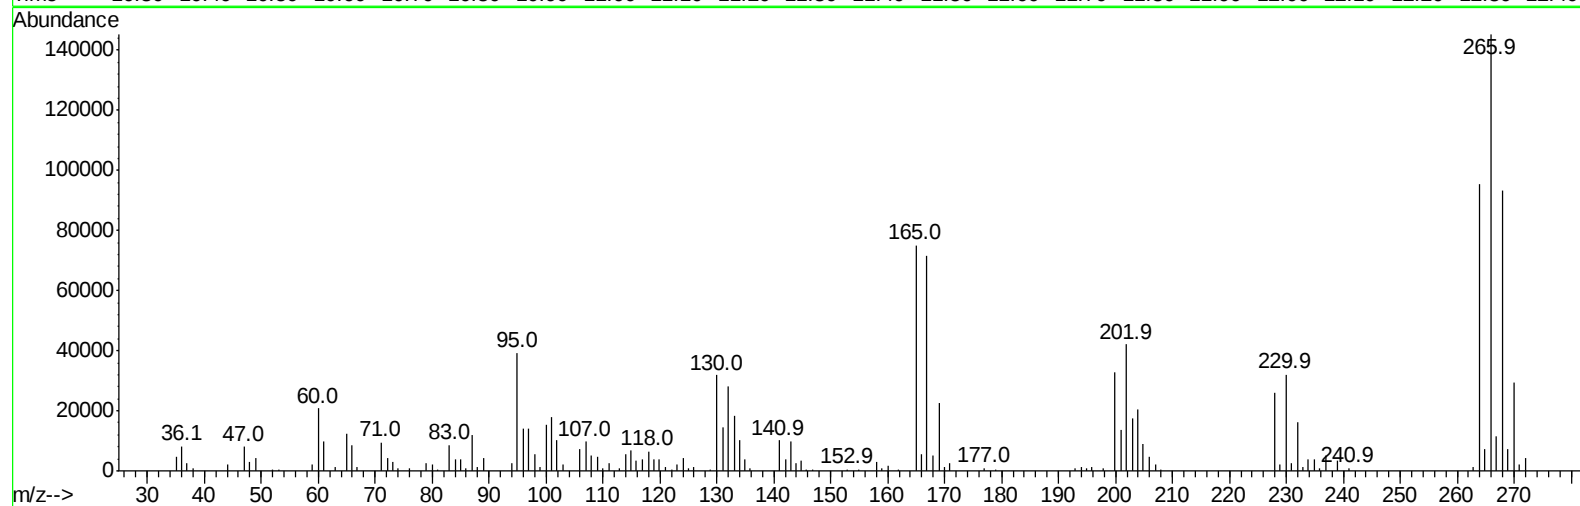


Data Path : Z:\HPCHEM1\BNA F\DATA\BF012617\
Data File : BF092508.D
Acq On : 26 Jan 2017 7:07
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 17:22:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

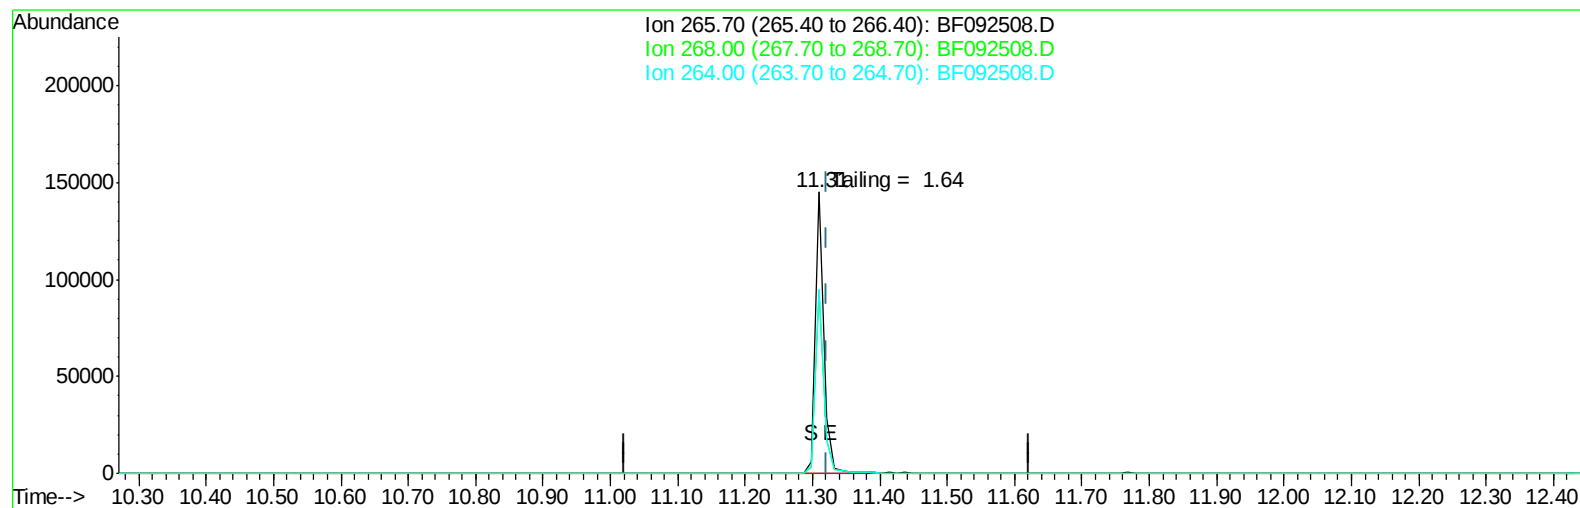

TIC: BF092508.D

(69) Pentachlorophenol (C)



11.310min (-0.012) 38348.07ng

response 129118

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.34
264.00	62.90	65.58
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012617\
Data File : BF092508.D
Acq On : 26 Jan 2017 7:07
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 17:22:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

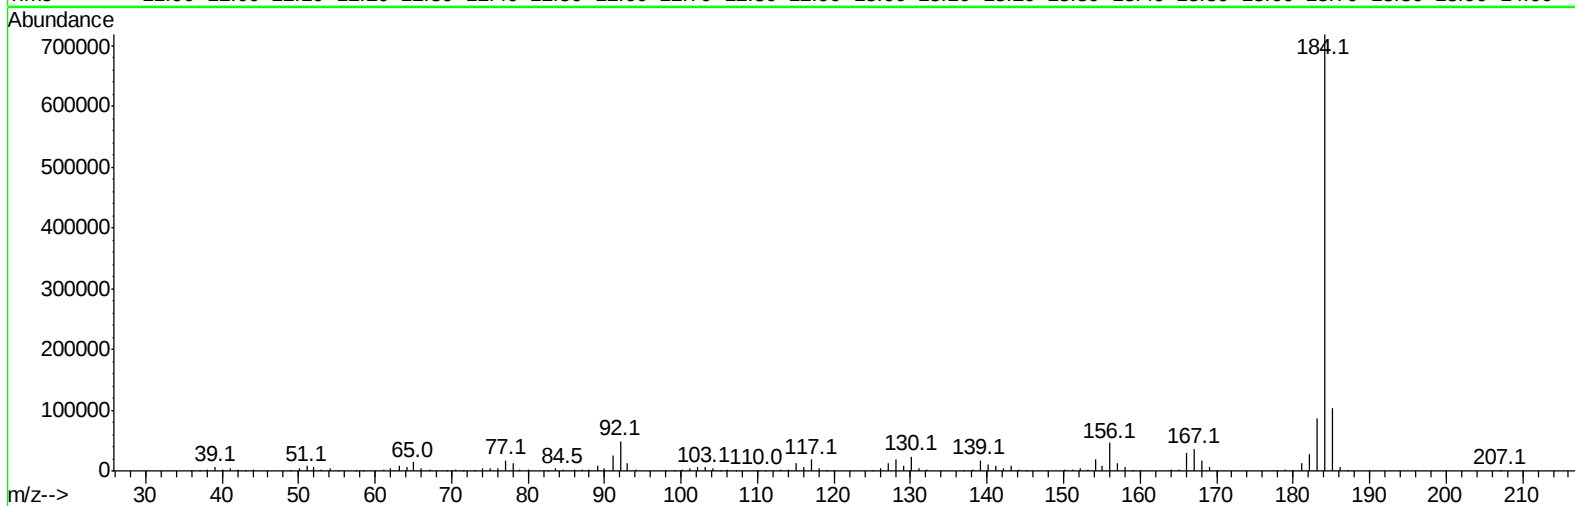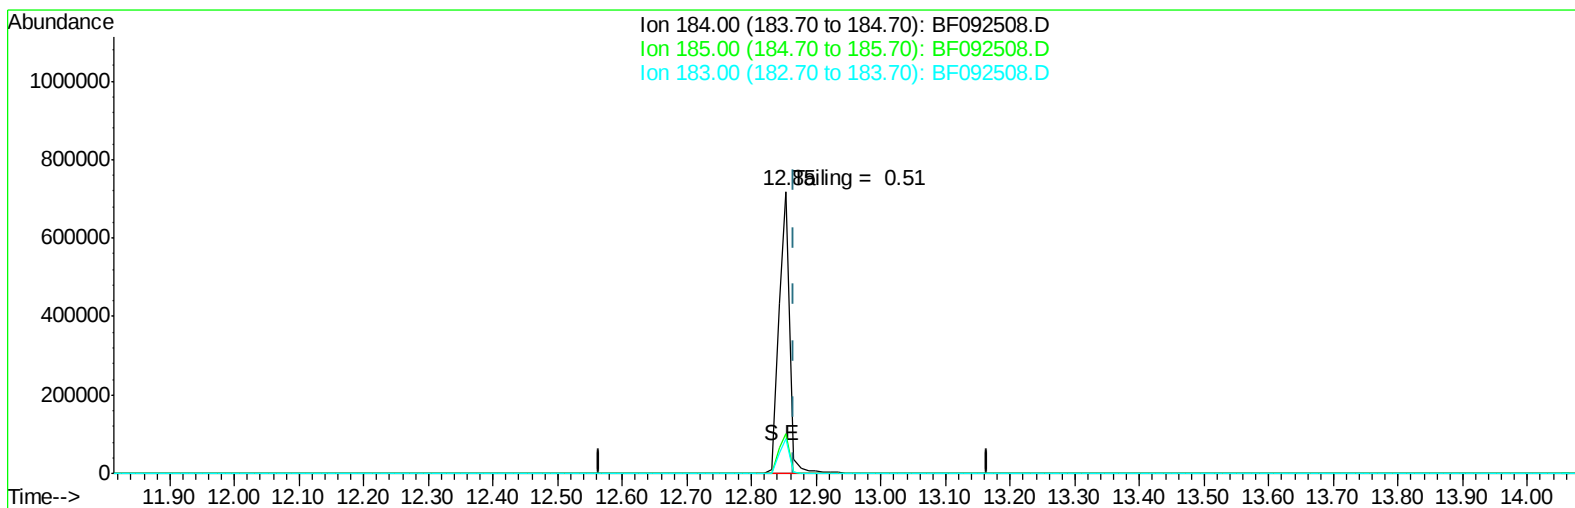

TIC: BF092508.D

(76) Benzidine

12.853min (-0.012) 0.00ng

response 851072

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.28
183.00	11.50	12.07
0.00	0.00	0.00