
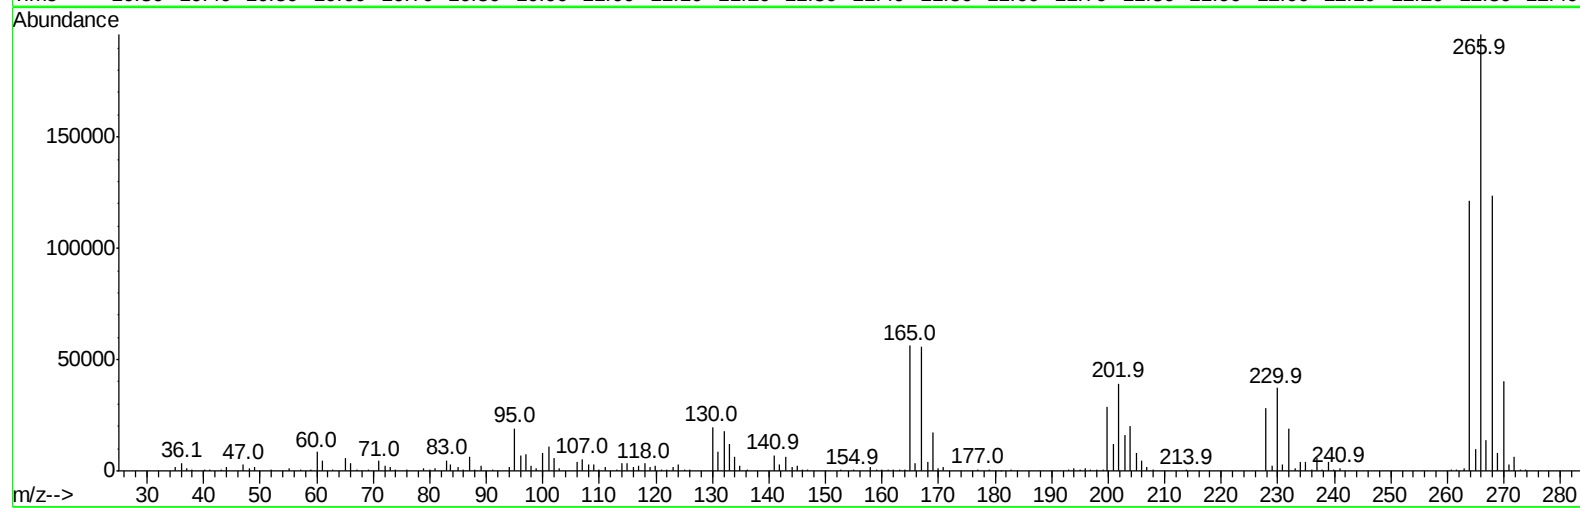


Data Path : Z:\HPCHEM1\BNA F\DATA\BF012617\
Data File : BF092531.D
Acq On : 26 Jan 2017 18:08
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 17:22:12 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

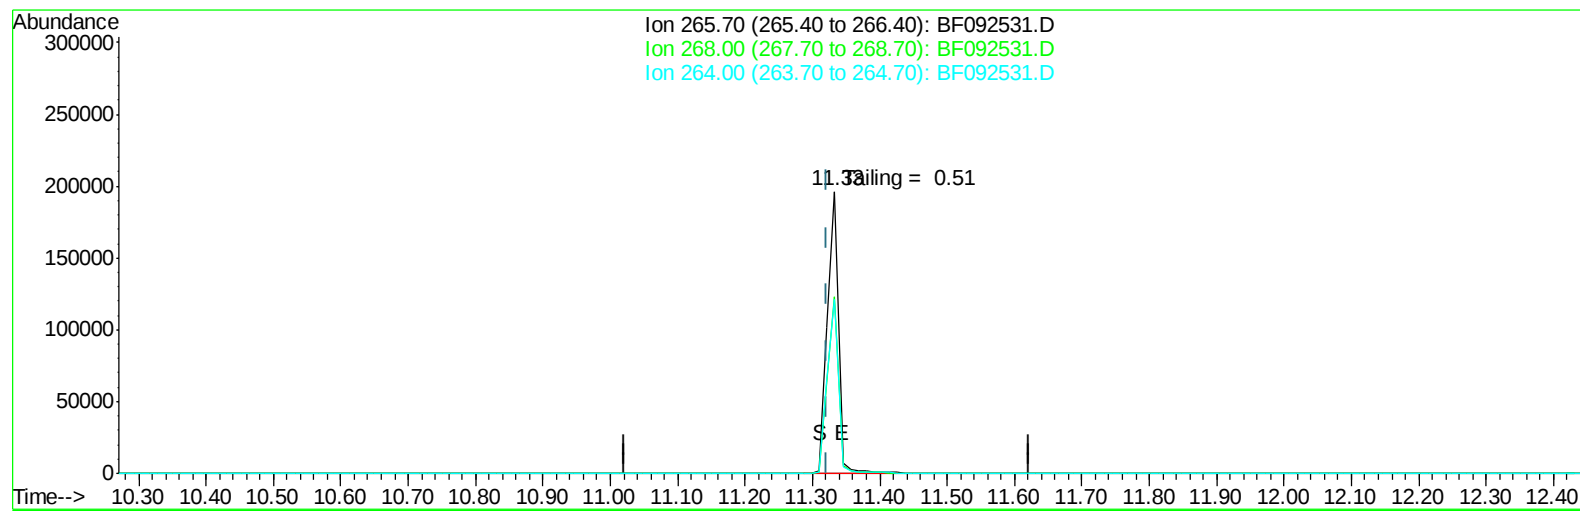

TIC: BF092531.D

(69) Pentachlorophenol (C)



11.333min (+0.011) 160656.32ng

response 217001

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.93
264.00	62.90	61.88
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF012617\
Data File : BF092531.D
Acq On : 26 Jan 2017 18:08
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 17:22:12 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

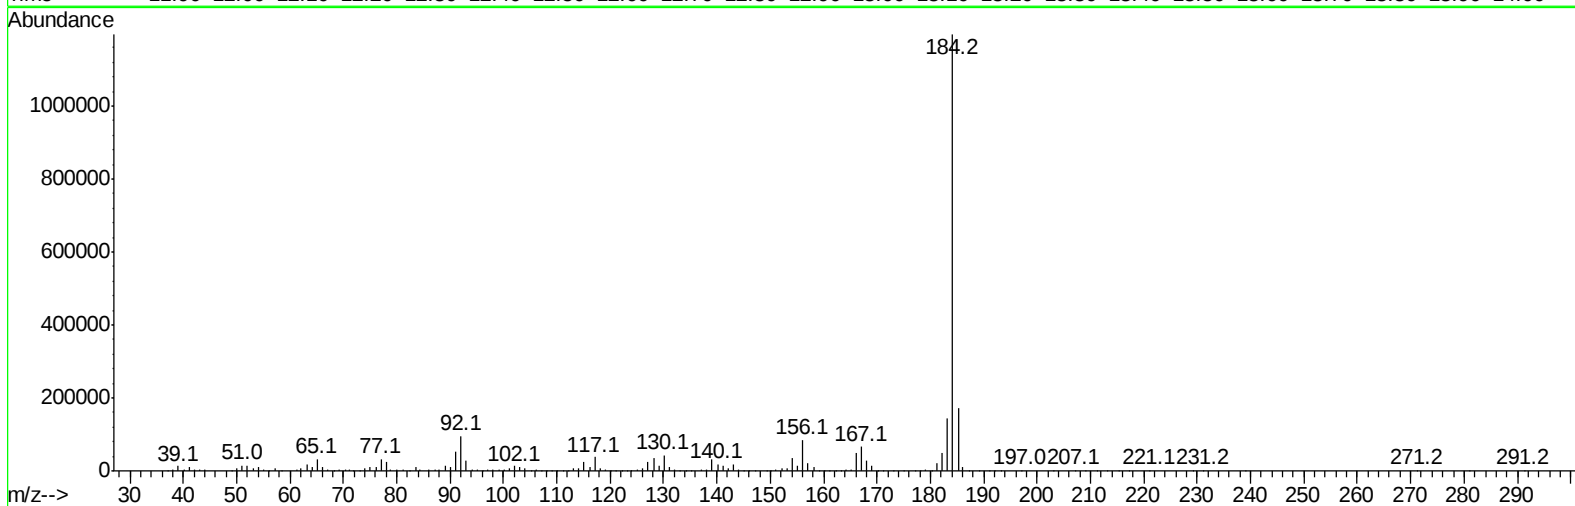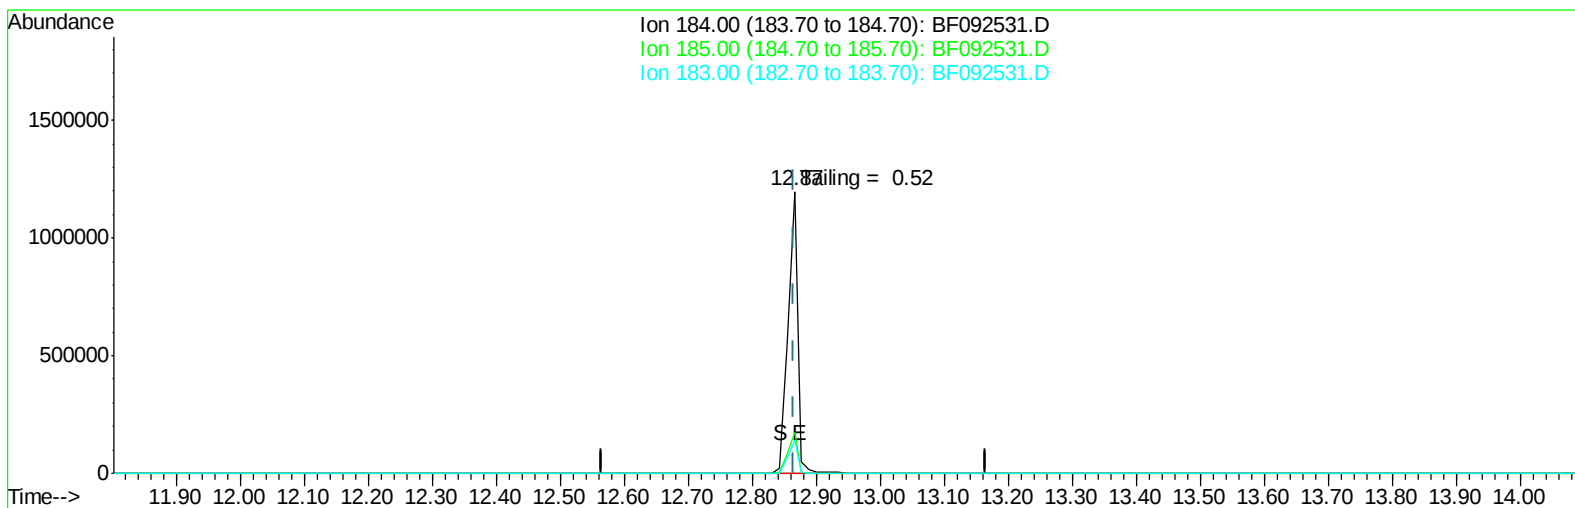

TIC: BF092531.D

(76) Benzidine

12.865min (-0.000) 34211.28ng

response 1282733

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.38
183.00	11.50	12.04
0.00	0.00	0.00