


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012617\
 Data File : BF092555.D
 Acq On : 27 Jan 2017 5:10
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 24 13:48:07 2017

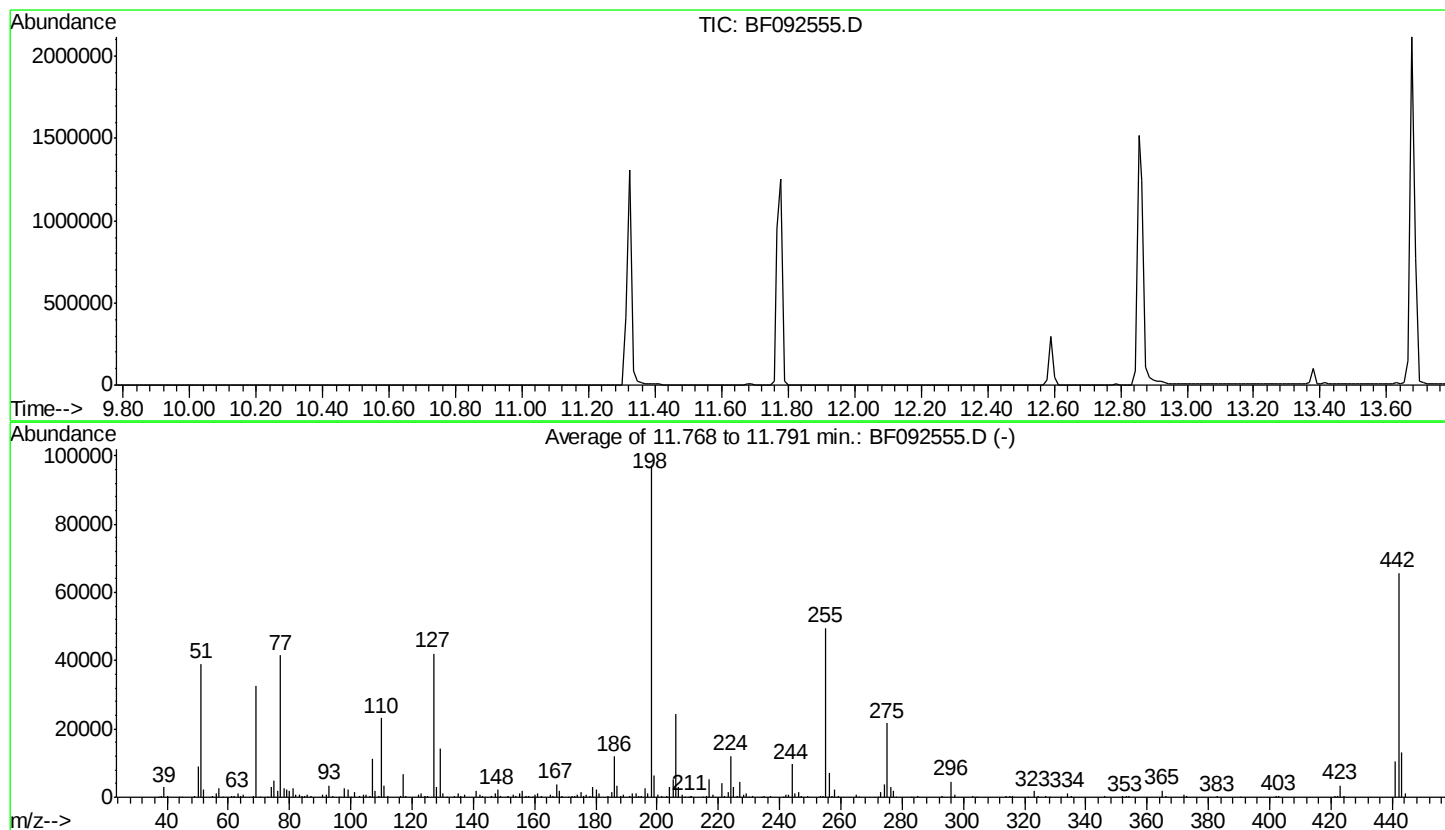

AutoFind: Scans 847, 848, 849; Background Corrected with Scan 843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	39101	PASS
68	69	0.00	2	1.8	573	PASS
69	198	0.00	100	33.5	32516	PASS
70	69	0.00	2	0.4	118	PASS
127	198	10	80	43.3	42053	PASS
197	198	0.00	2	1.0	963	PASS
198	198	100	100	100.0	97098	PASS
199	198	5	9	6.5	6288	PASS
275	198	10	60	22.3	21656	PASS
365	198	1	100	2.1	1995	PASS
441	442	0.01	24	15.7	10347	PASS
442	198	50	100	67.7	65748	PASS
443	442	15	24	19.8	12987	PASS