
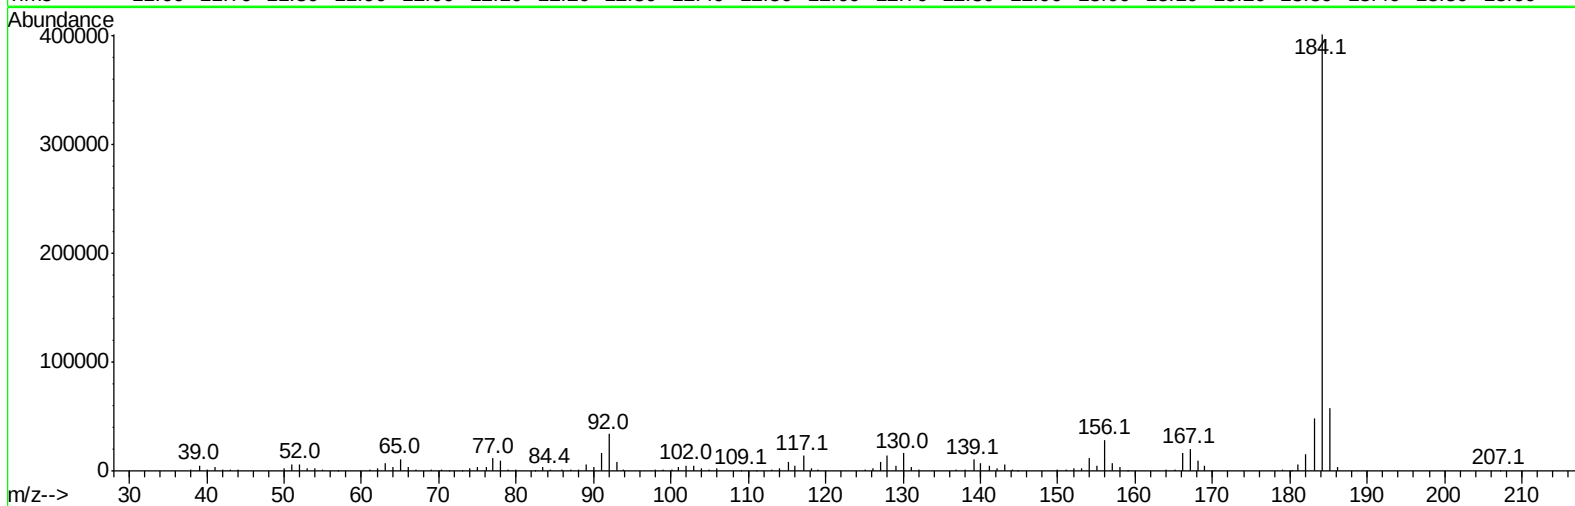


Data Path : U:\HPCHEM1\BNA F\DATA\BF012618\
Data File : BF102462.D
Acq On : 26 Jan 2018 11:51
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 05:42:02 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 16:18:07 2018
Response via : Initial Calibration

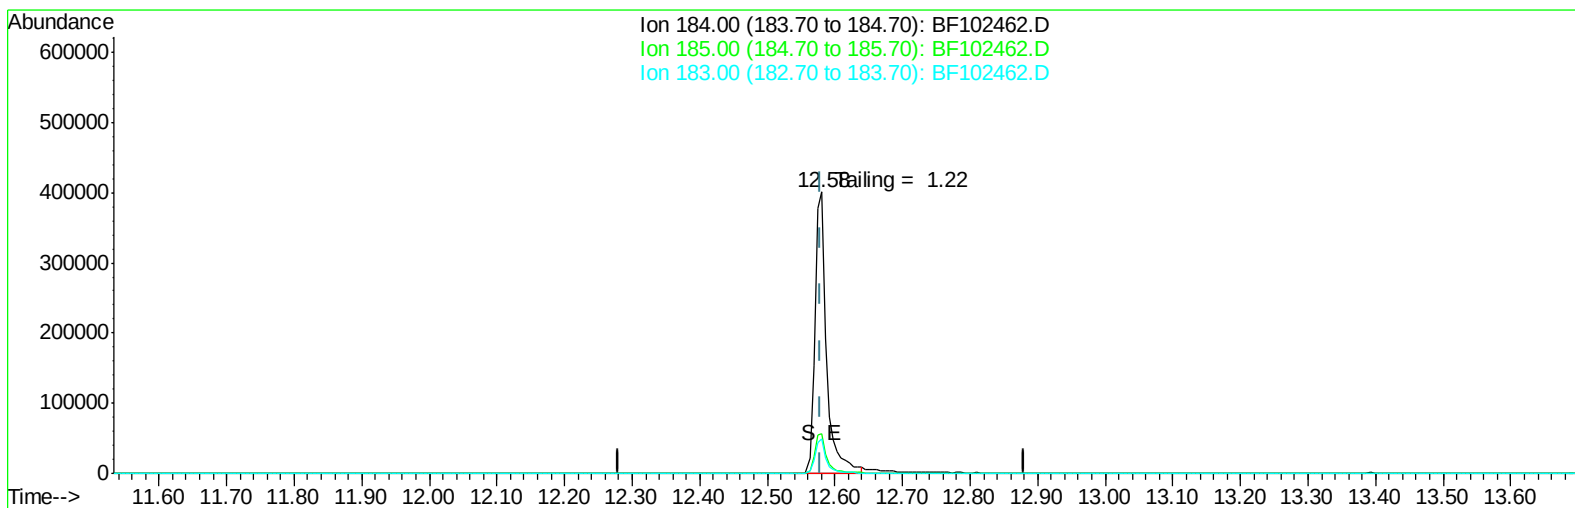

TIC: BF102462.D

(76) Benzidine



12.580min (-0.000) 0.00ng

response 504143

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.32
183.00	11.60	12.14
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF012618\
Data File : BF102462.D
Acq On : 26 Jan 2018 11:51
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 05:42:02 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 16:18:07 2018
Response via : Initial Calibration

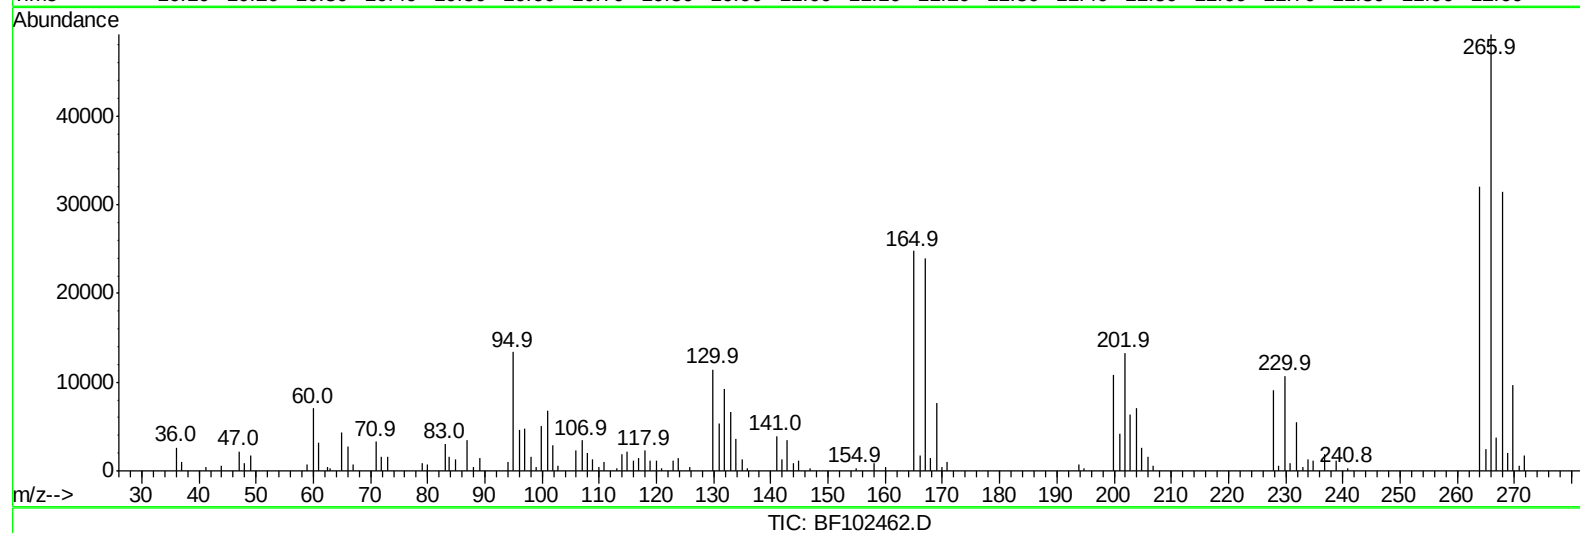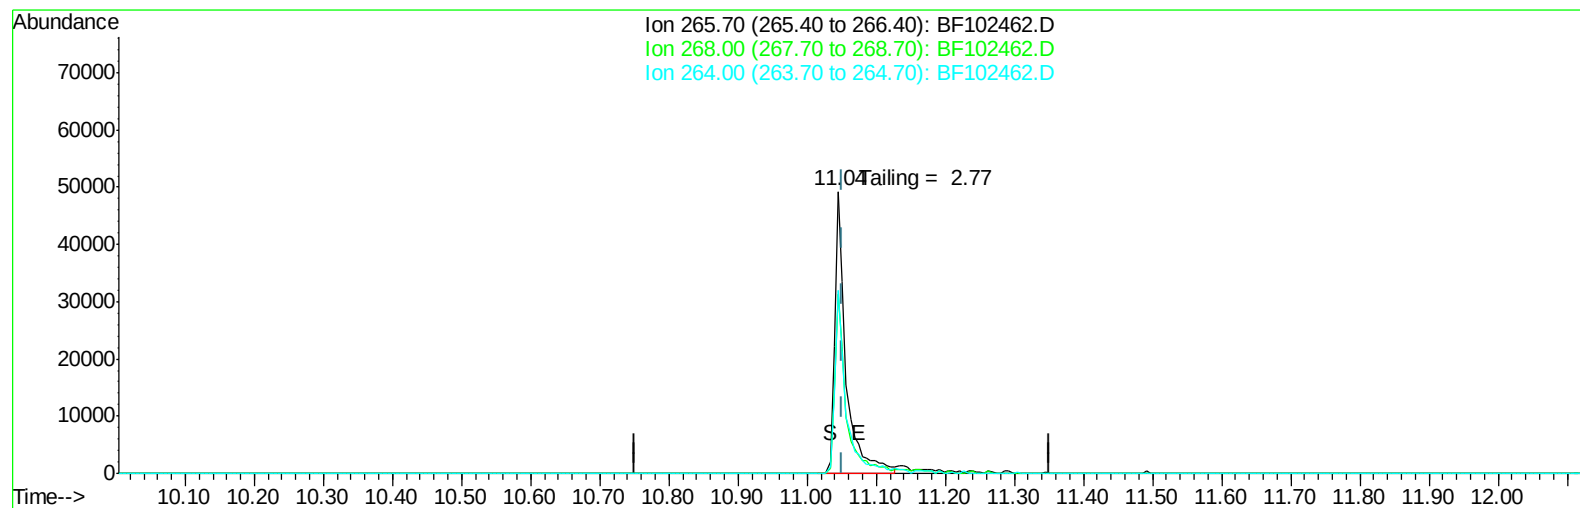

(69) Pentachlorophenol (C)

11.045min (-0.006) 26020.87ng

response 56447

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.84
264.00	61.90	65.06
0.00	0.00	0.00