
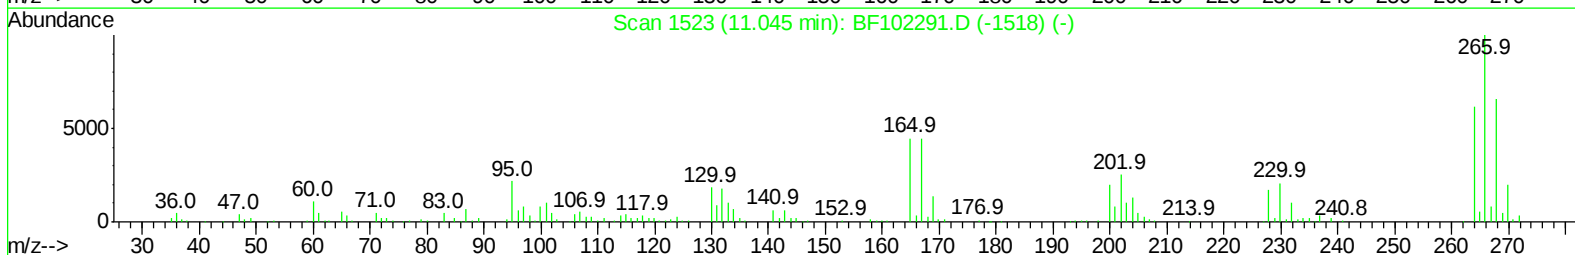
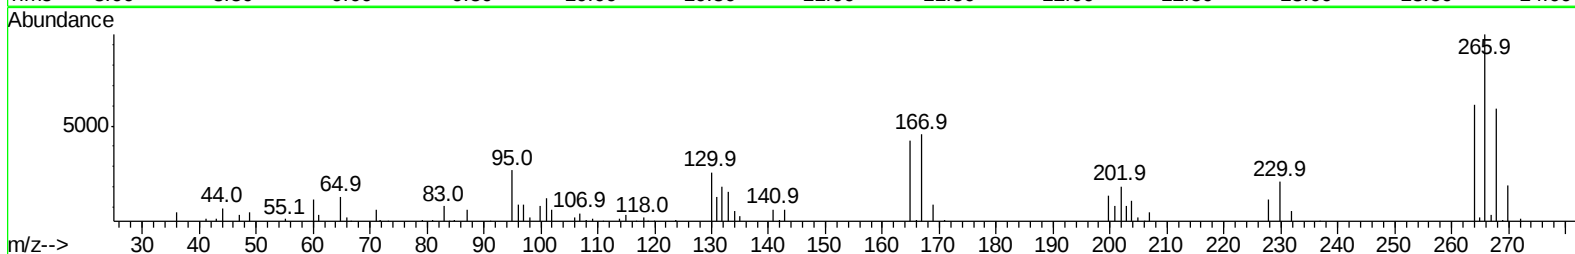


Data Path : U:\HPCHEM1\BNA F\DATA\BF012618\
Data File : BF102488.D
Acq On : 27 Jan 2018 1:00
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 05:43:48 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 16:18:07 2018
Response via : Initial Calibration

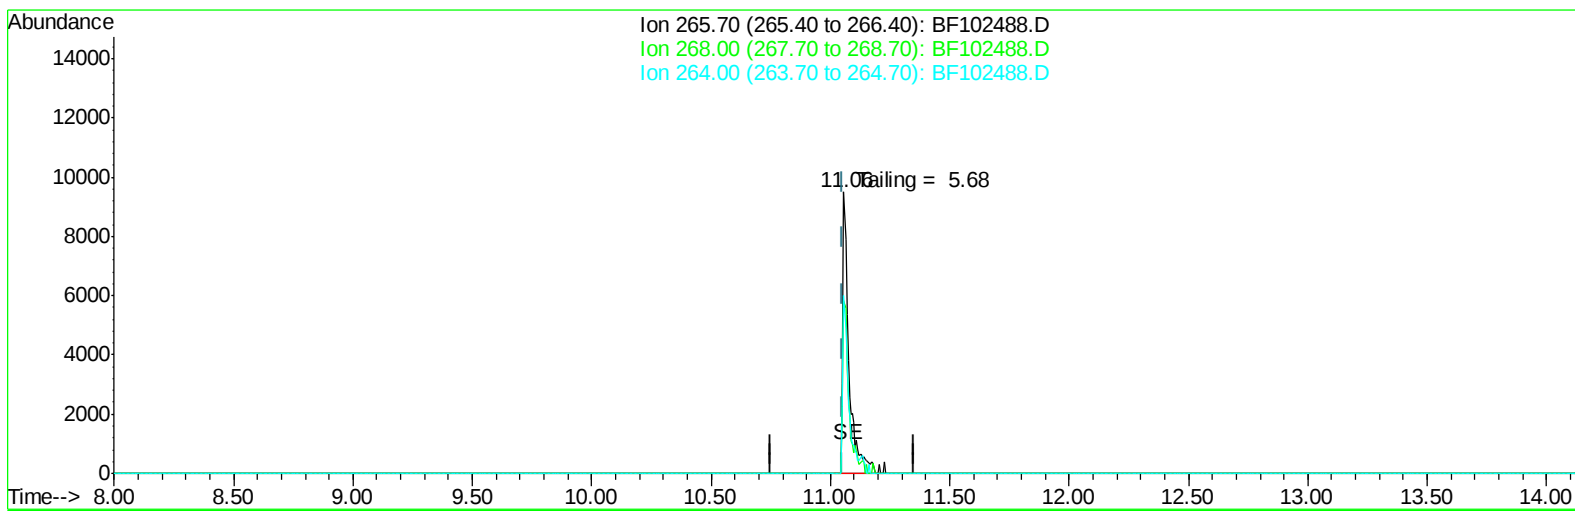

TIC: BF102488.D

(69) Pentachlorophenol (C)




11.057min (+0.006) 5535.54ng m

response 14844

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.33
264.00	61.90	63.31
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF012618\
Data File : BF102488.D
Acq On : 27 Jan 2018 1:00
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 05:43:48 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 26 16:18:07 2018
Response via : Initial Calibration

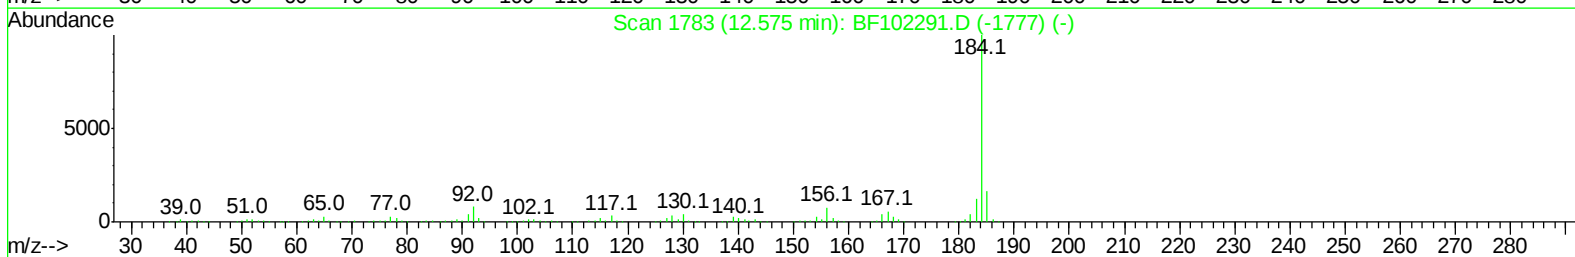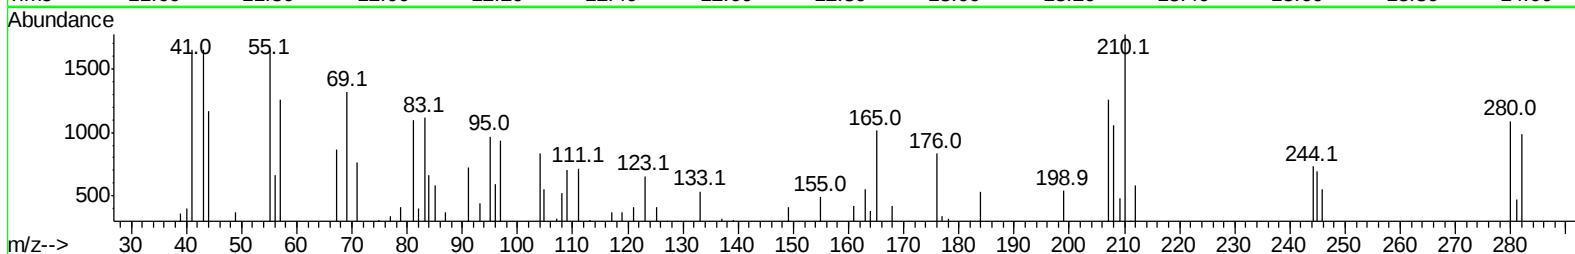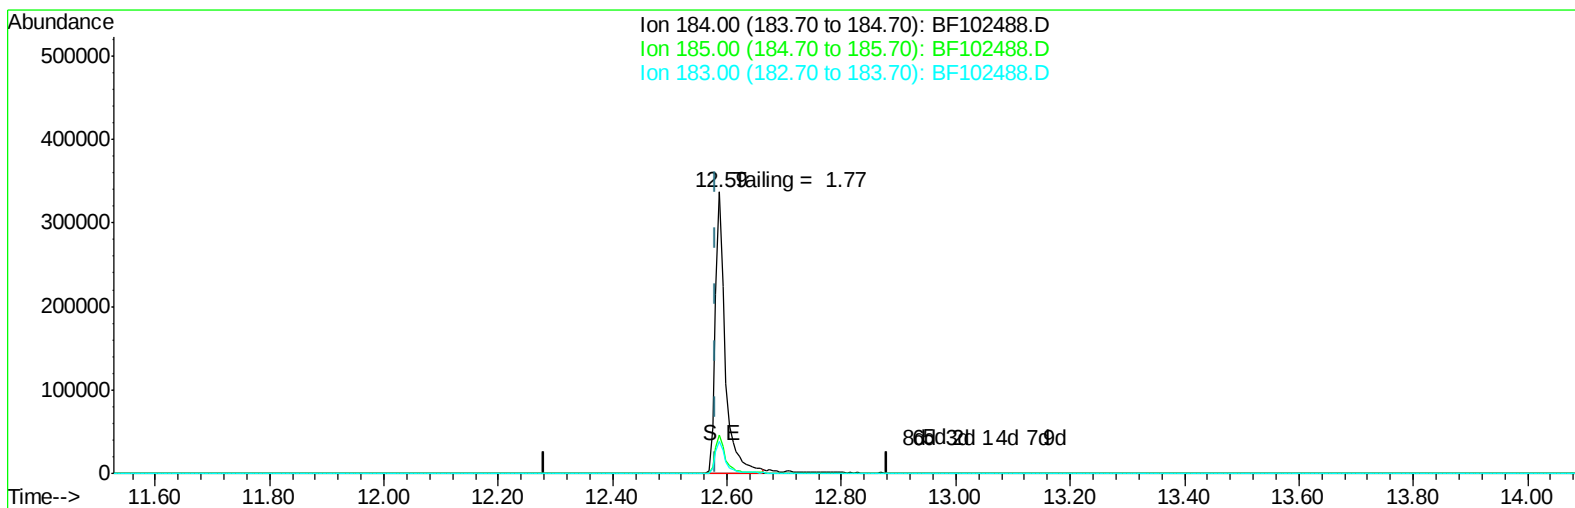

TIC: BF102488.D

(76) Benzidine

13.057min (+0.477) 137.94ng

response 1089

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00