


Data Path : U:\HPCHEM1\BNA_F\Data\BF012618\
 Data File : BF102462.D
 Acq On : 26 Jan 2018 11:51
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 27 20:48:40 2018

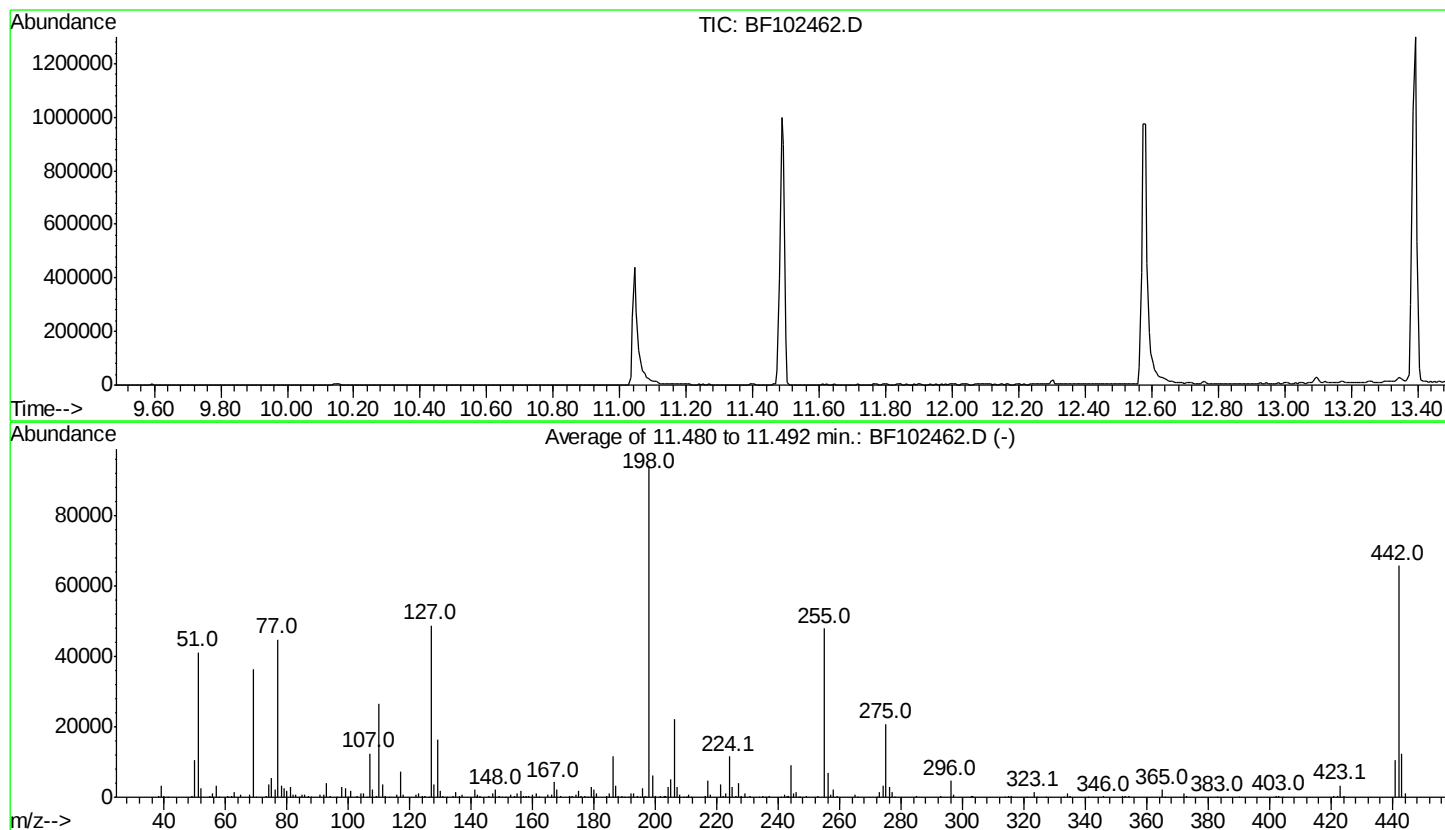

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.7	41170	PASS
68	69	0.00	2	1.8	668	PASS
69	198	0.00	100	38.7	36418	PASS
70	69	0.00	2	0.3	127	PASS
127	198	10	80	51.8	48741	PASS
197	198	0.00	2	0.6	553	PASS
198	198	100	100	100.0	94130	PASS
199	198	5	9	6.7	6269	PASS
275	198	10	60	22.1	20799	PASS
365	198	1	100	2.1	2023	PASS
441	443	0.01	100	83.9	10414	PASS
442	198	50	100	69.8	65663	PASS
443	442	15	24	18.9	12406	PASS