


Data Path : U:\HPCHEM1\BNA_F\Data\BF012618\
 Data File : BF102488.D
 Acq On : 27 Jan 2018 1:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jan 27 20:48:40 2018

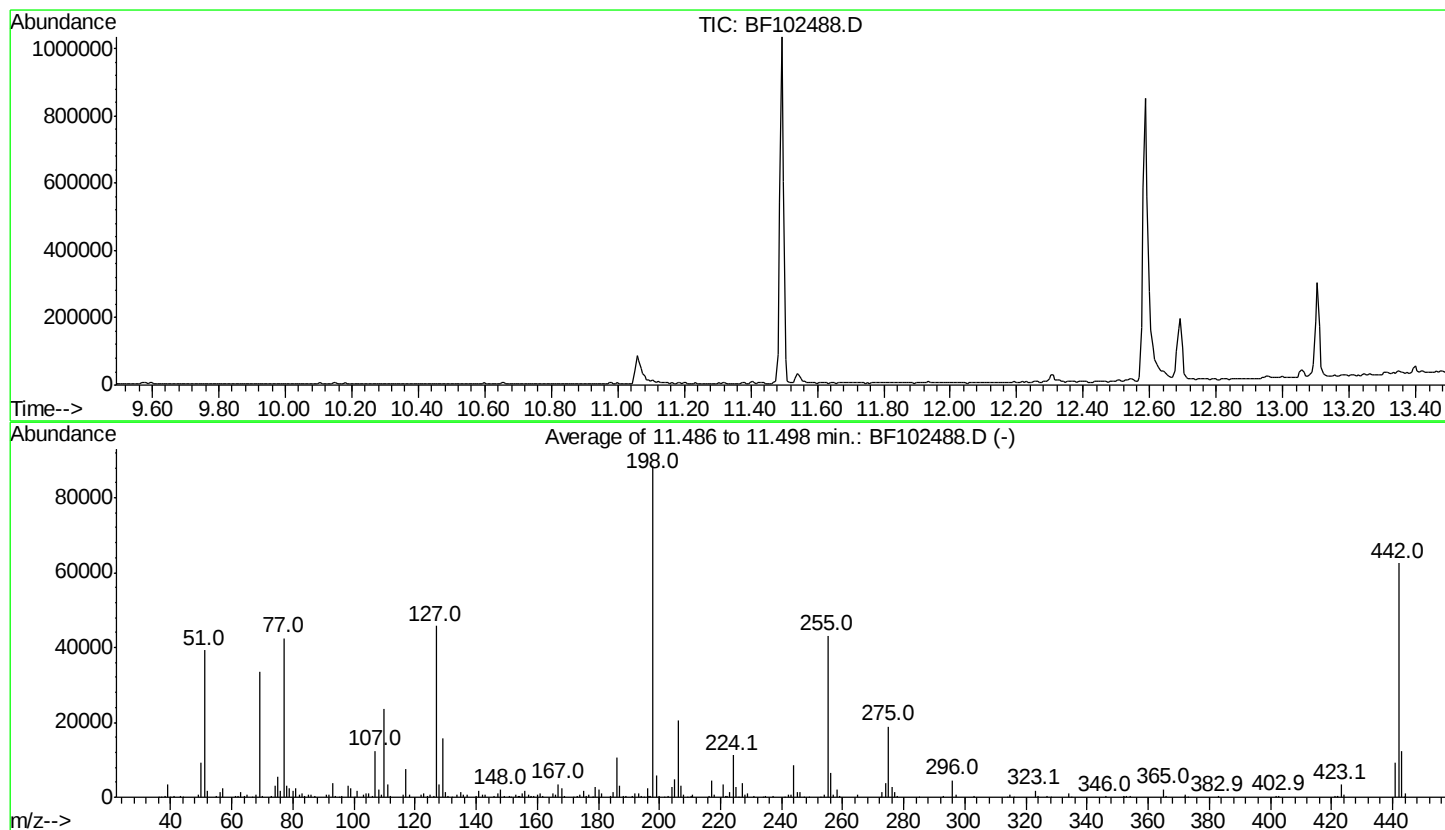

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	39274	PASS
68	69	0.00	2	2.0	657	PASS
69	198	0.00	100	38.0	33660	PASS
70	69	0.00	2	0.7	250	PASS
127	198	10	80	51.6	45741	PASS
197	198	0.00	2	0.4	340	PASS
198	198	100	100	100.0	88560	PASS
199	198	5	9	6.7	5966	PASS
275	198	10	60	21.4	18919	PASS
365	198	1	100	2.5	2228	PASS
441	443	0.01	100	75.8	9347	PASS
442	198	50	100	70.5	62450	PASS
443	442	15	24	19.7	12332	PASS