


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012716\
 Data File : BF084616.D
 Acq On : 27 Jan 2016 8:48
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 25 16:24:07 2016

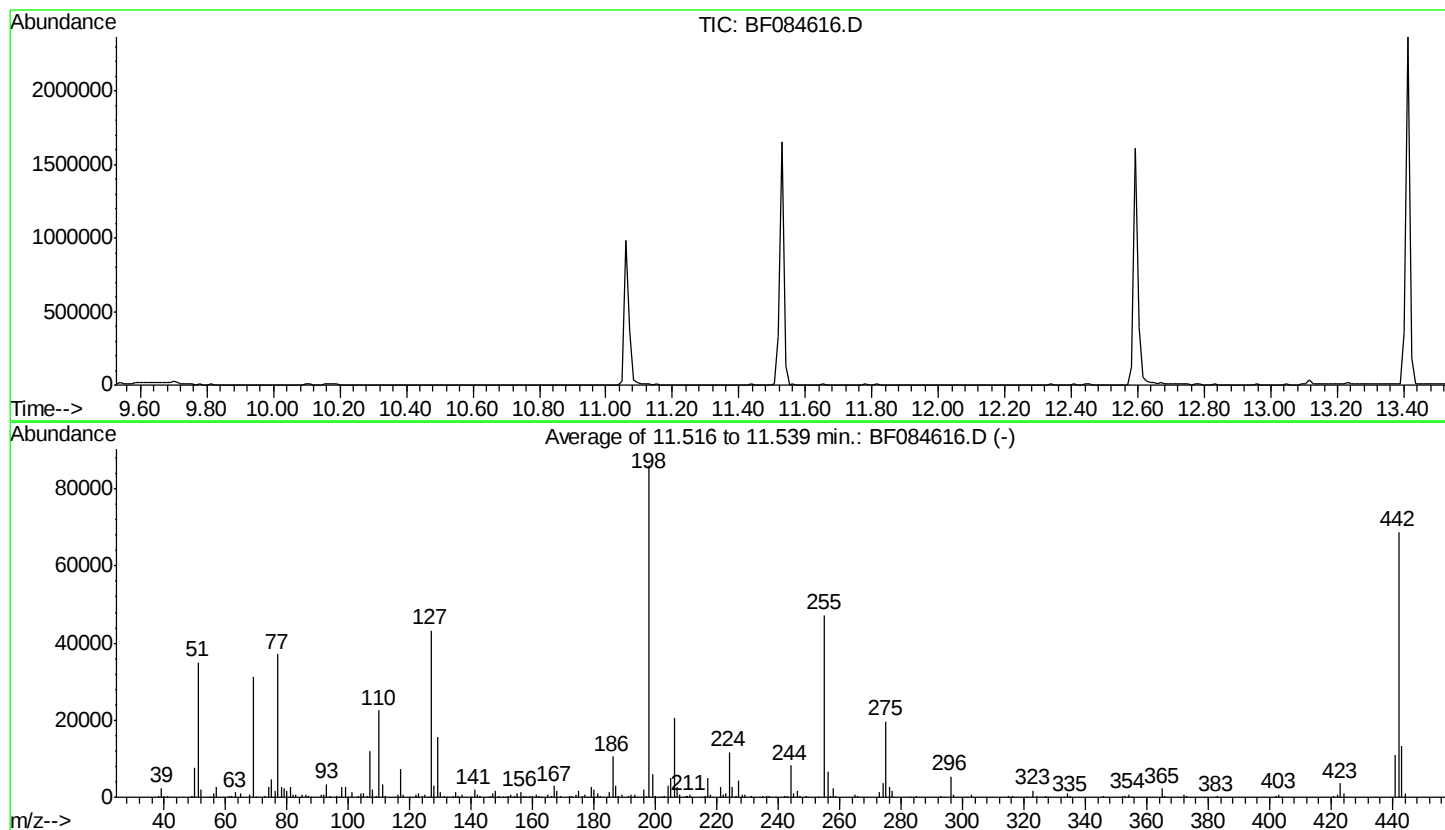

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	34887	PASS
68	69	0.00	2	1.8	576	PASS
69	198	0.00	100	36.4	31287	PASS
70	69	0.00	2	0.5	141	PASS
127	198	10	80	50.2	43204	PASS
197	198	0.00	2	0.5	426	PASS
198	198	100	100	100.0	86056	PASS
199	198	5	9	6.8	5840	PASS
275	198	10	60	23.0	19768	PASS
365	198	1	100	2.6	2273	PASS
441	442	0.01	24	15.9	10925	PASS
442	198	50	100	79.9	68801	PASS
443	442	15	24	19.3	13297	PASS