

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012717\
 Data File : BF092615.D
 Acq On : 28 Jan 2017 9:44
 Operator : SJ/MA
 Sample : I1528-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-16-COMP

Quant Time: Jan 29 23:47:32 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 24 13:48:07 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	149614	20.00	ng	0.00
21) Naphthalene-d8	8.26	136	574705	20.00	ng	-0.01
38) Acenaphthene-d10	10.03	164	277902	20.00	ng	0.00
63) Phenanthrene-d10	11.53	188	376628	20.00	ng	0.00
75) Chrysene-d12	14.16	240	311082	20.00	ng	-0.01
86) Perylene-d12	15.65	264	212929	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	1372107	142.69	ng	0.05
7) Phenol-d6	6.62	99	1858716	151.74	ng	0.03
23) Nitrobenzene-d5	7.54	82	907836	86.29	ng	0.00
41) 2,4,6-Tribromophenol	10.83	330	232763	122.91	ng	0.01
44) 2-Fluorobiphenyl	9.36	172	1688717	112.37	ng	0.00
78) Terphenyl-d14	13.12	244	1126534	96.43	ng	0.00
Target Compounds						
10) Phenol	6.64	94	69856	4.72	ng	# 62
19) n-Nitroso-di-n-propylamine	7.54	70	121679	14.59	ng	# 83
25) Isophorone	7.54	82	895333	43.19	ng	# 65
49) Dimethylphthalate	9.74	163	171449	9.70	ng	100
56) 2,4-Dinitrotoluene	10.03	165	35084	7.32	ng	# 19
64) 4,6-Dinitro-2-methylphenol	10.83	198	680	5.25	ng	# 1
66) 4-Bromophenyl-phenylether	10.83	248	17412	4.58	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012717\
Data File : BF092615.D
Acq On : 28 Jan 2017 9:44
Operator : SJ/MA
Sample : I1528-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-16-COMP

Quant Time: Jan 29 23:47:32 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

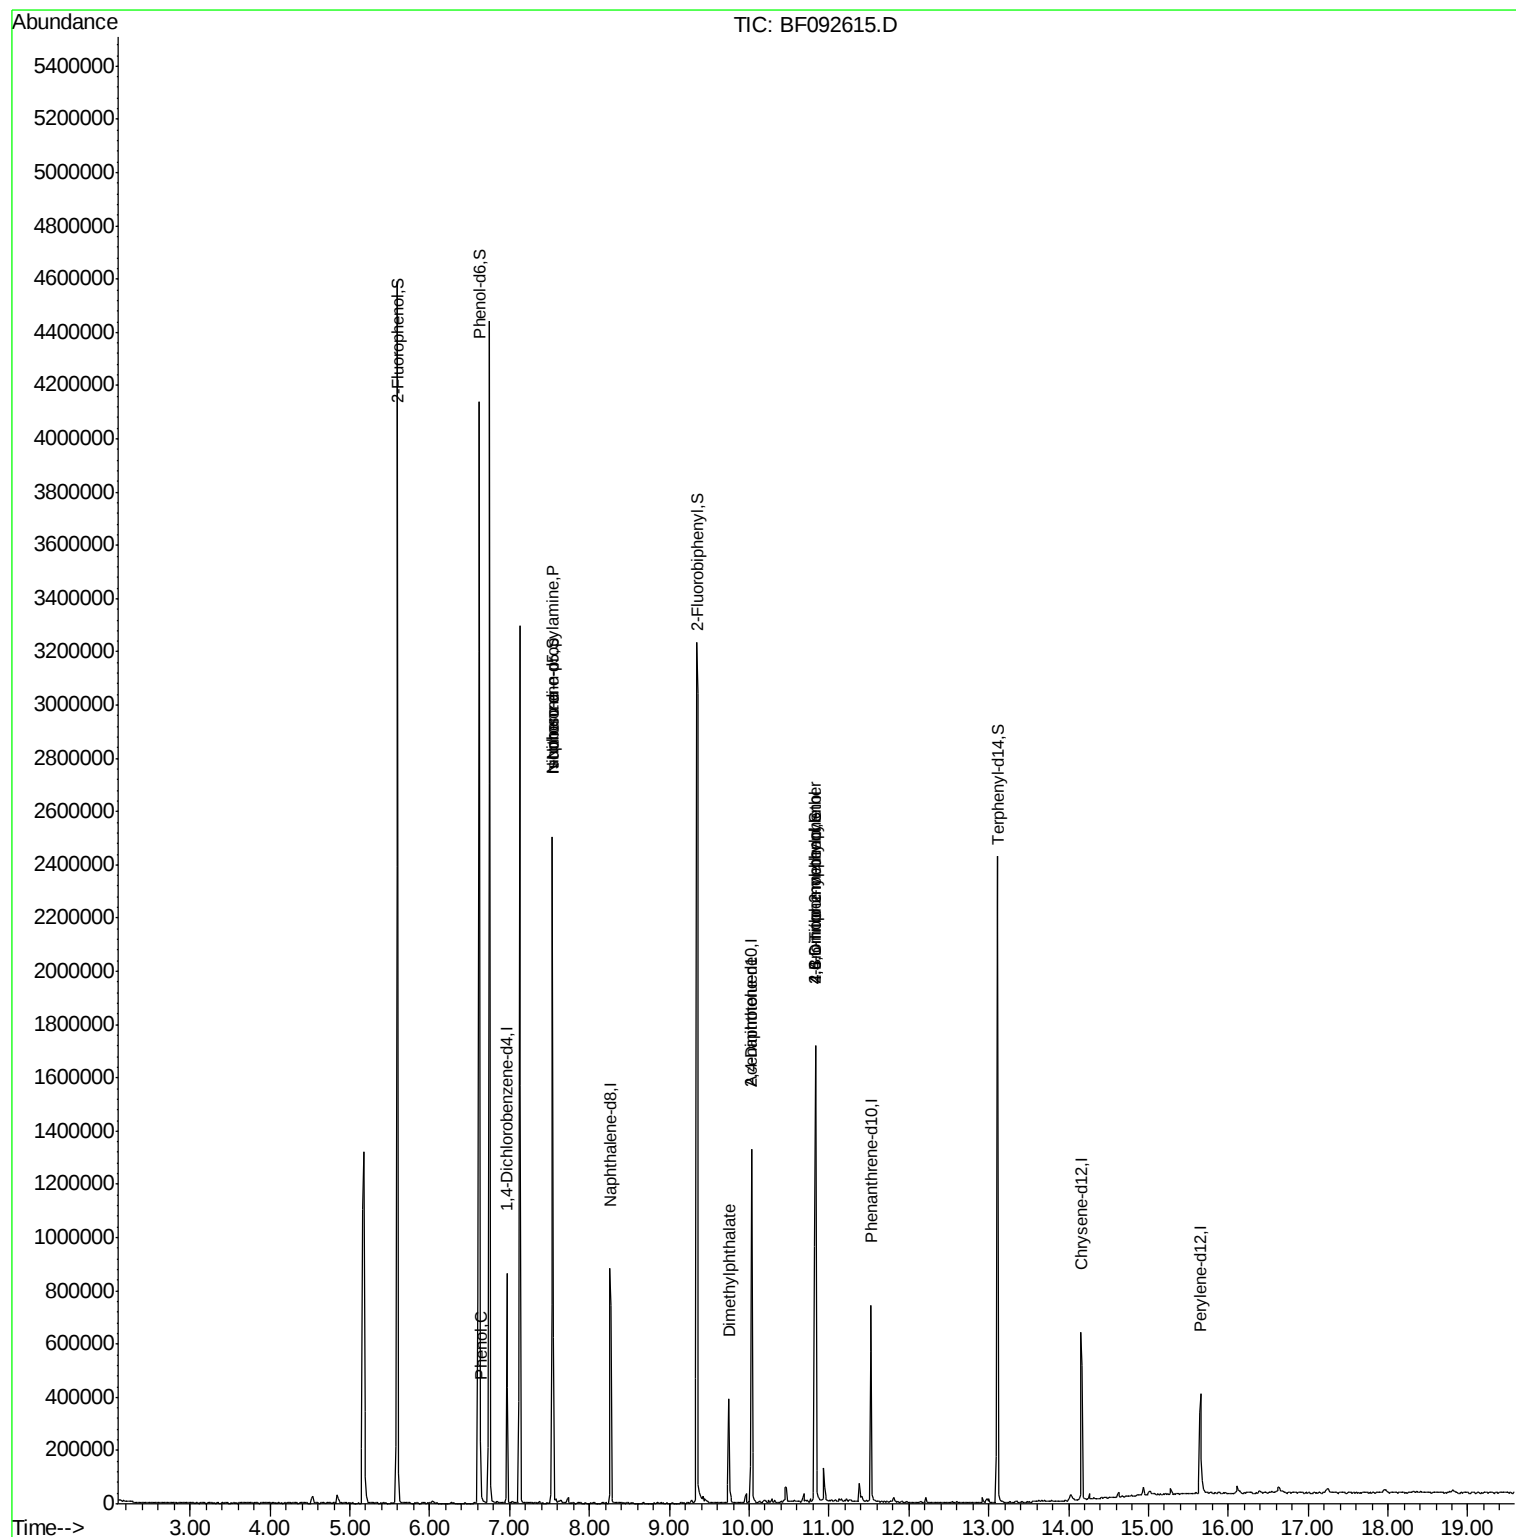



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.97 min Scan# 427

Delta R.T. -0.00 min

Lab File: BF092615.D

Acq: 28 Jan 2017 9:44

Instrument :

BNA_F

ClientSampleId :

SB-16-COMP


Tgt Ion:152 Resp: 149614

Ion Ratio Lower Upper

152 100

150 156.3 124.9 187.3




115 68.6 46.0 69.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

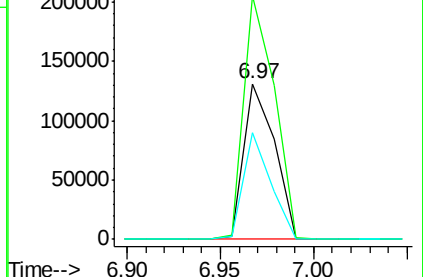

#5

2-Fluorophenol

Concen: 142.69 ng

RT: 5.60 min Scan# 307

Delta R.T. 0.05 min

Lab File: BF092615.D

Acq: 28 Jan 2017 9:44


Tgt Ion:112 Resp: 1372107

Ion Ratio Lower Upper

112 100

64 63.9 46.1 69.1



63 32.8 23.8 35.6




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

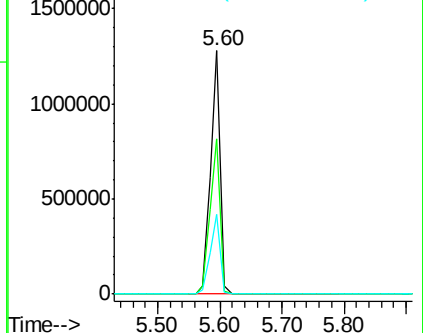

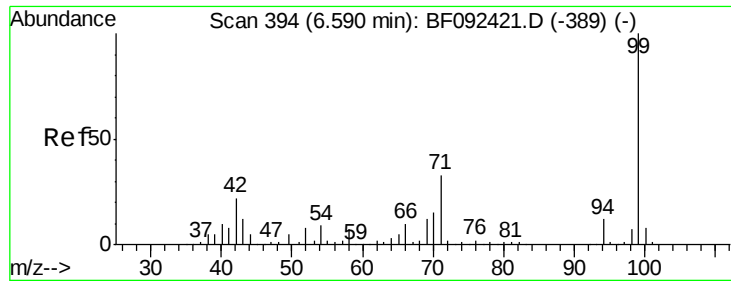

#7

Phenol-d6

Concen: 151.74 ng

RT: 6.62 min Scan# 397

Delta R.T. 0.03 min

Lab File: BF092615.D

Acq: 28 Jan 2017 9:44

Instrument :

BNA_F

ClientSampleId :

SB-16-COMP


Tgt Ion: 99 Resp: 1858716

Ion Ratio Lower Upper




99 100

42 19.1 15.6 23.4

71 32.6 27.5 41.3



Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

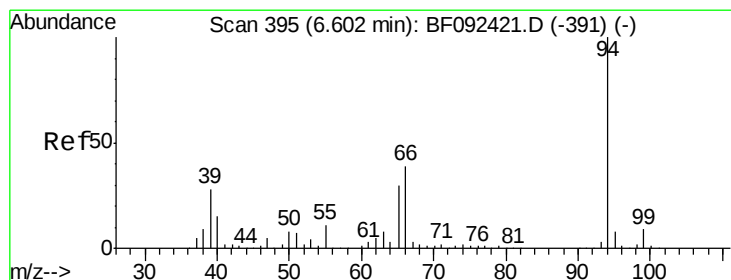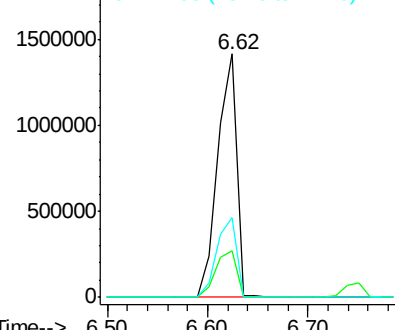

#10

Phenol

Concen: 4.72 ng

RT: 6.64 min Scan# 398

Delta R.T. 0.03 min

Lab File: BF092615.D

Acq: 28 Jan 2017 9:44


Tgt Ion: 94 Resp: 69856

Ion Ratio Lower Upper



94 100

65 22.4 21.4 61.4

66 30.3 44.0 84.0#



Abundance Ion 94.00 (93.70 to 94.70): BF0
Ion 65.00 (64.70 to 65.70): BF0
Ion 66.00 (65.70 to 66.70): BF0

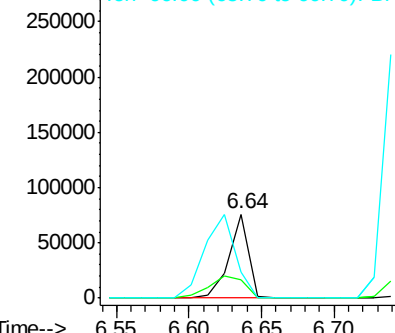



#19

n-Nitroso-di-n-propylamine

Concen: 14.59 ng

RT: 7.54 min Scan# 477

Delta R.T. 0.15 min

Lab File: BF092615.D

Acq: 28 Jan 2017 9:44

Instrument :

BNA_F

ClientSampleId :

SB-16-COMP

Tgt Ion: 70 Resp: 121679


Ion Ratio Lower Upper

70 100

42 54.0 49.4 74.0

101 0.0 7.4 11.2#

130 1.9 14.2 21.4#



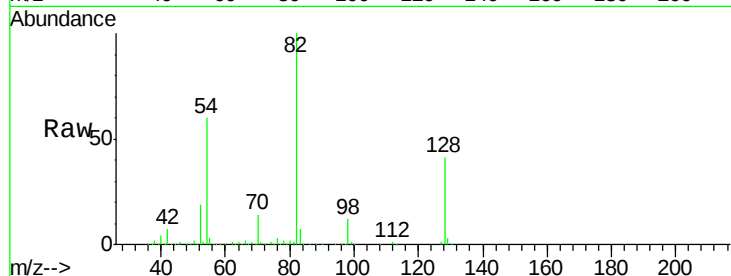


Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

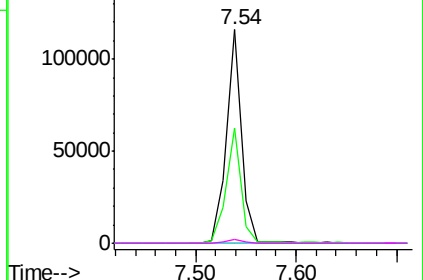

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.26 min Scan# 540

Delta R.T. -0.01 min

Lab File: BF092615.D

Acq: 28 Jan 2017 9:44

Tgt Ion: 136 Resp: 574705


Ion Ratio Lower Upper

136 100

137 11.3 8.4 12.6

54 13.5 4.5 6.7#

68 8.9 3.6 5.4#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



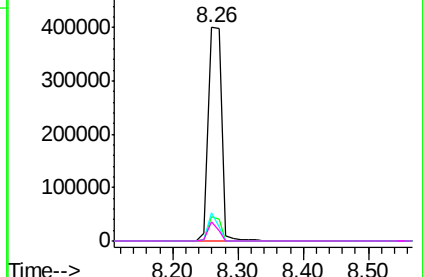





#23
 Nitrobenzene-d5
 Concen: 86.29 ng
 RT: 7.54 min Scan# 477
 Delta R.T. -0.00 min
 Lab File: BF092615.D
 Acq: 28 Jan 2017 9:44




Instrument :
 BNA_F
 ClientSampleId :
 SB-16-COMP


Tgt Ion: 82 Resp: 907836
 Ion Ratio Lower Upper
 82 100
 128 40.7 34.6 52.0
 54 59.5 39.5 59.3#

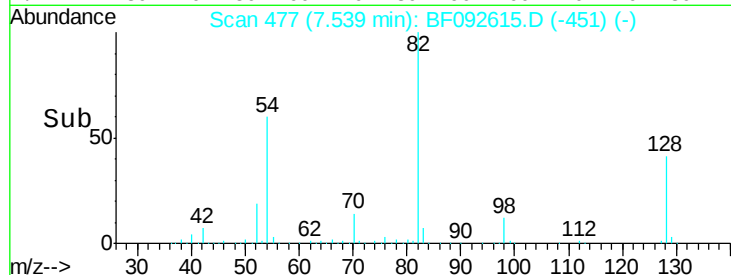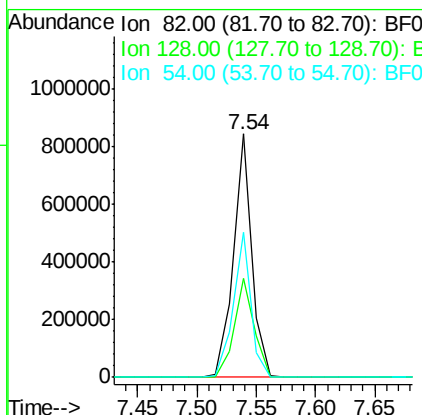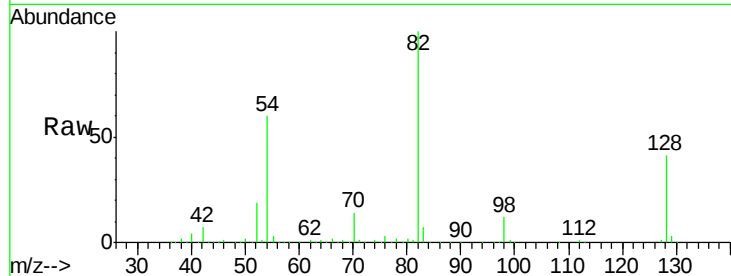

#25
 Isophorone
 Concen: 43.19 ng
 RT: 7.54 min Scan# 477
 Delta R.T. -0.26 min
 Lab File: BF092615.D
 Acq: 28 Jan 2017 9:44

Tgt Ion: 82 Resp: 895333
 Ion Ratio Lower Upper
 82 100
 95 0.0 5.6 8.4#
 138 0.0 14.6 22.0#



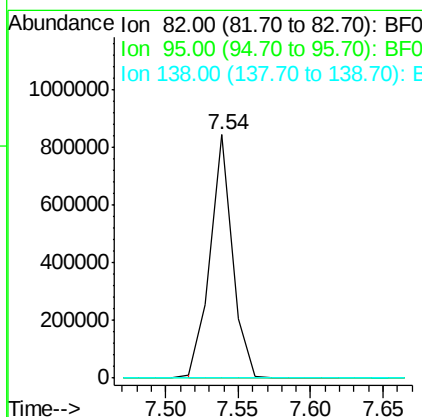



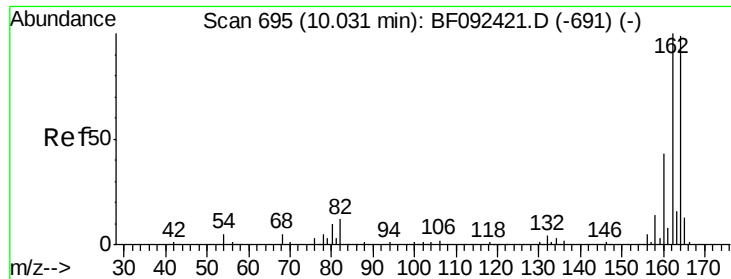

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.03 min Scan# 695
 Delta R.T. -0.00 min
 Lab File: BF092615.D
 Acq: 28 Jan 2017 9:44




Instrument :
 BNA_F
 ClientSampleId :
 SB-16-COMP


Tgt Ion:164 Resp: 277902
 Ion Ratio Lower Upper
 164 100
 162 101.8 80.2 120.2
 160 42.6 36.9 55.3

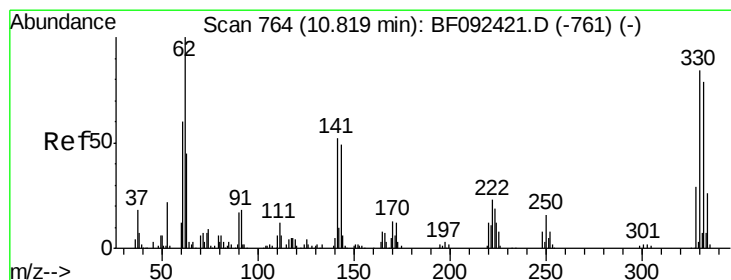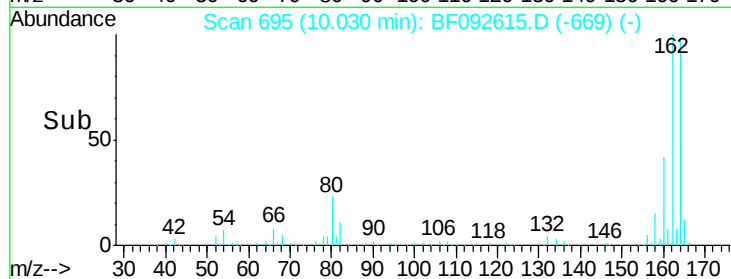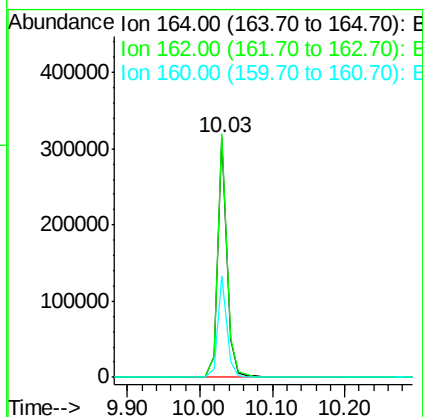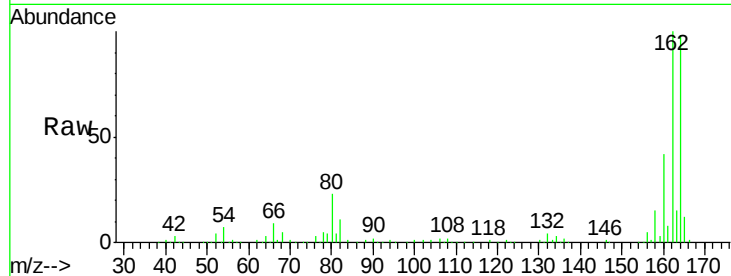

#41
 2,4,6-Tribromophenol
 Concen: 122.91 ng
 RT: 10.83 min Scan# 765
 Delta R.T. 0.01 min
 Lab File: BF092615.D
 Acq: 28 Jan 2017 9:44

Tgt Ion:330 Resp: 232763
 Ion Ratio Lower Upper
 330 100
 332 96.7 77.4 116.2
 141 37.9 34.1 51.1



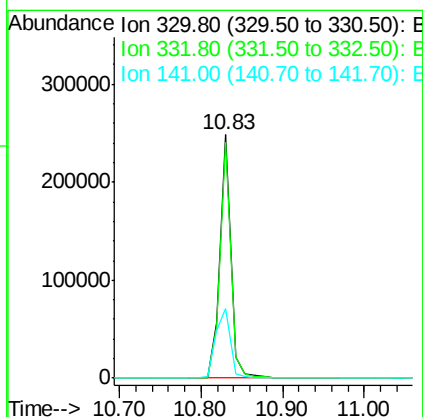





#44
 2-Fluorobiphenyl
 Concen: 112.37 ng
 RT: 9.36 min Scan# 636
 Delta R.T. -0.00 min
 Lab File: BF092615.D
 Acq: 28 Jan 2017 9:44




Instrument :
 BNA_F
 ClientSampleId :
 SB-16-COMP


Tgt Ion:172 Resp: 1688717
 Ion Ratio Lower Upper
 172 100
 171 36.0 29.4 44.0
 170 24.3 20.2 30.4

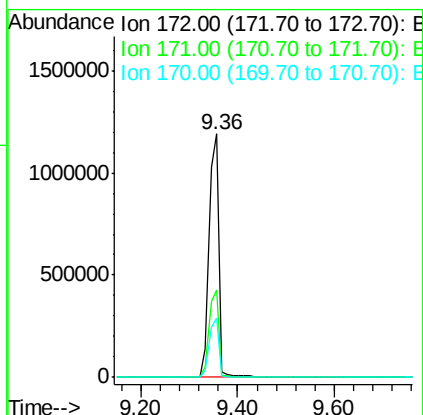

#49
 Dimethylphthalate
 Concen: 9.70 ng
 RT: 9.74 min Scan# 670
 Delta R.T. -0.01 min
 Lab File: BF092615.D
 Acq: 28 Jan 2017 9:44

Tgt Ion:163 Resp: 171449
 Ion Ratio Lower Upper
 163 100
 194 3.6 3.0 4.4
 164 9.9 8.0 12.0



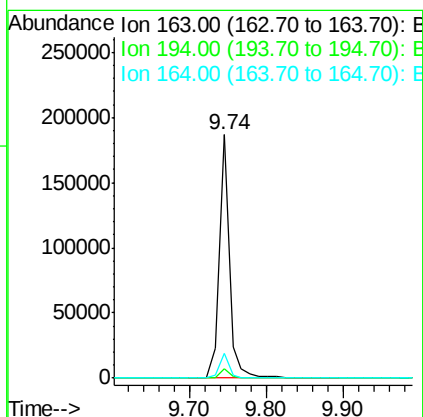



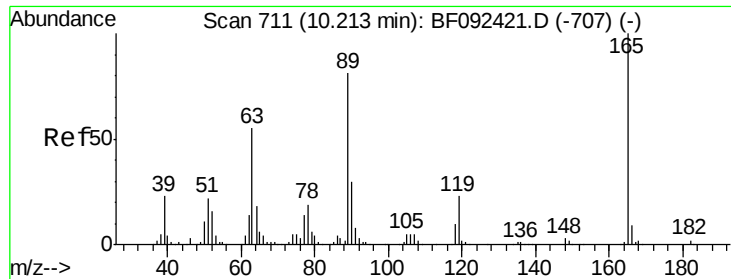

#56
2,4-Dinitrotoluene
Concen: 7.32 ng
RT: 10.03 min Scan# 695
Delta R.T. -0.18 min
Lab File: BF092615.D
Acq: 28 Jan 2017 9:44




Instrument :
BNA_F
ClientSampleId :
SB-16-COMP


Tgt Ion:	165	Resp:	35084
Ion	Ratio	Lower	Upper
165	100		
63	0.9	40.2	60.4#
89	0.0	62.5	93.7#
182	0.0	1.8	2.8#

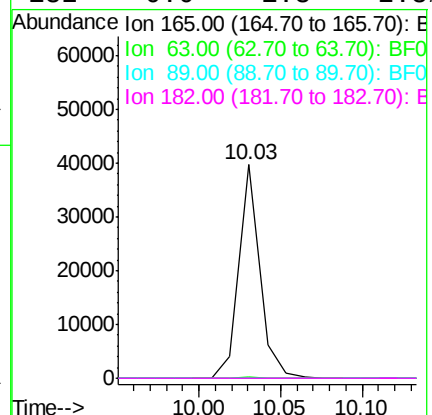

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.53 min Scan# 826
Delta R.T. -0.00 min
Lab File: BF092615.D
Acq: 28 Jan 2017 9:44

Tgt Ion:	188	Resp:	376628
Ion	Ratio	Lower	Upper
188	100		
94	7.5	10.0	15.0#
80	7.2	11.2	16.8#

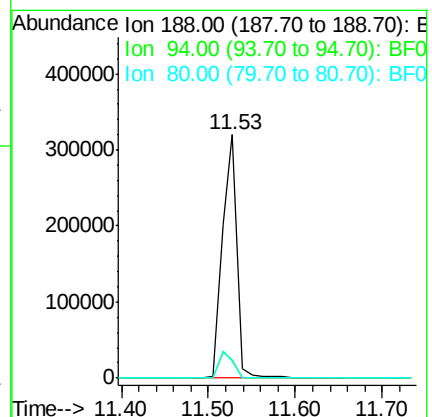

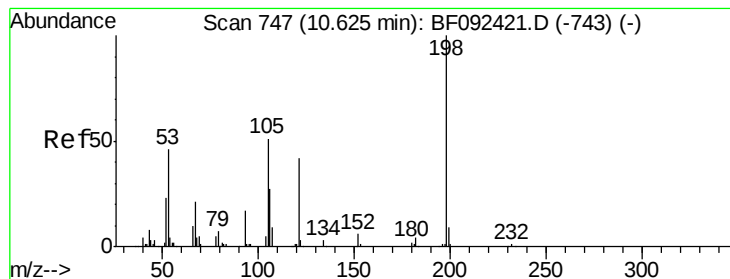

#64

4,6-Dinitro-2-methylphenol

Concen: 5.25 ng

RT: 10.83 min Scan# 765

Delta R.T. 0.21 min

Lab File: BF092615.D

Acq: 28 Jan 2017 9:44

Instrument :

BNA_F

ClientSampleId :

SB-16-COMP


Tgt Ion:198 Resp: 680

Ion Ratio Lower Upper

198 100

51 155.3 6.7 46.7#




105 166.3 16.6 56.6#

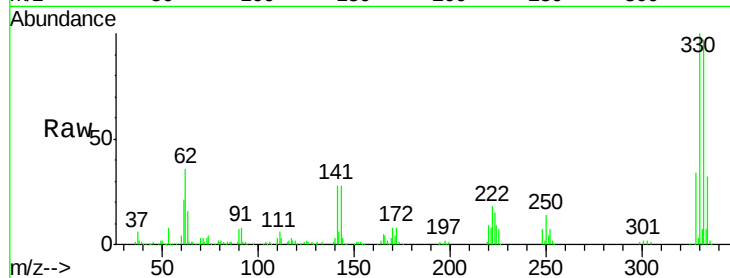

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF0

Ion 105.00 (104.70 to 105.70): E

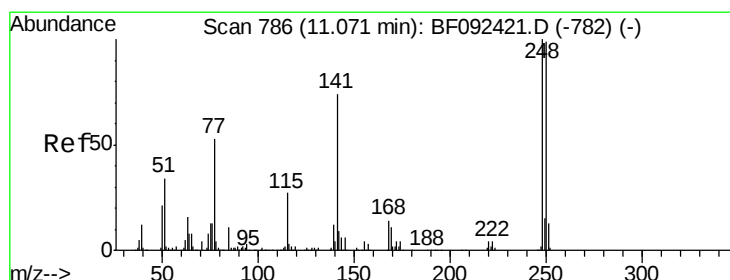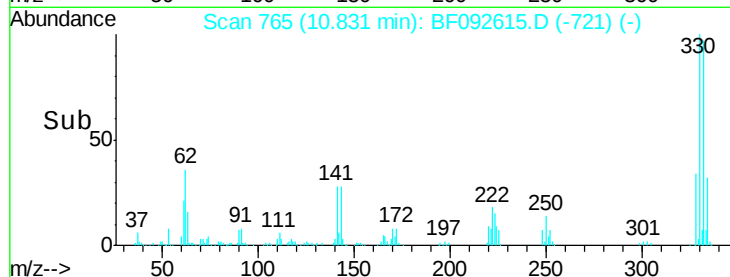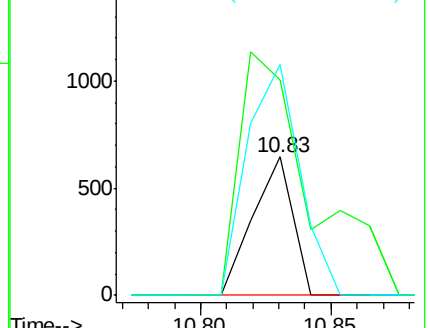

#66

4-Bromophenyl-phenylether

Concen: 4.58 ng

RT: 10.83 min Scan# 765

Delta R.T. -0.24 min

Lab File: BF092615.D

Acq: 28 Jan 2017 9:44


Tgt Ion:248 Resp: 17412

Ion Ratio Lower Upper

248 100

250 201.1 76.9 115.3#



141 397.6 68.2 102.4#

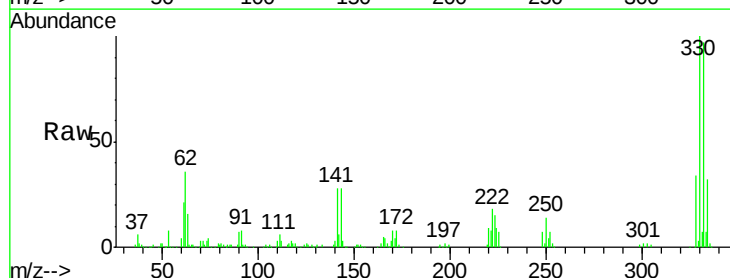


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

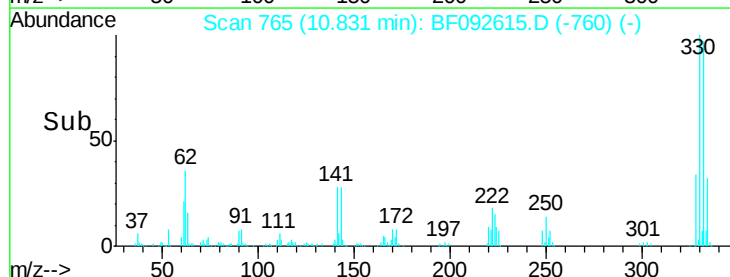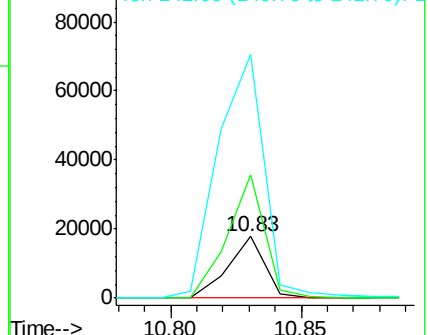

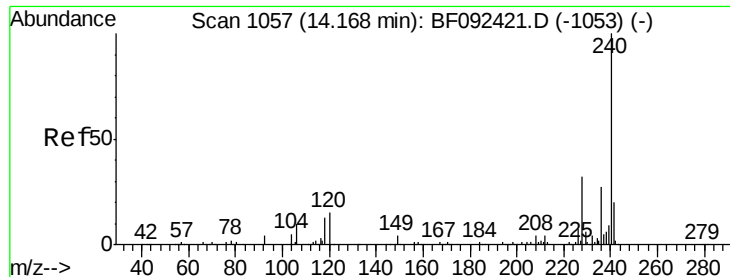

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.16 min Scan# 1056

Delta R.T. -0.01 min

Lab File: BF092615.D

Acq: 28 Jan 2017 9:44

Instrument :

BNA_F

ClientSampleId :

SB-16-COMP


Tgt Ion:240 Resp: 311082

Ion Ratio Lower Upper

240 100

120 18.5 12.9 19.3




236 26.5 20.9 31.3

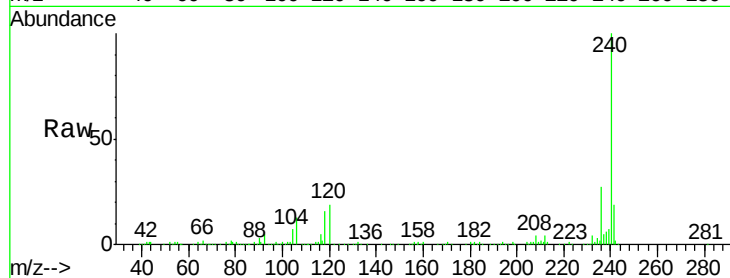

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

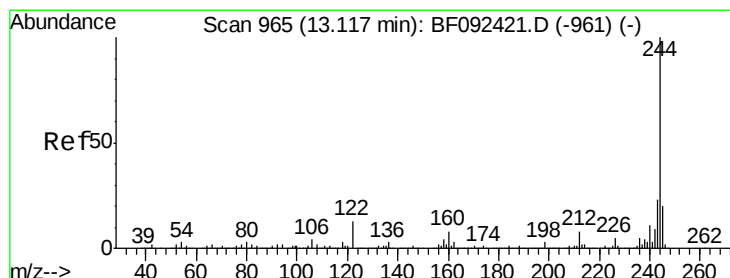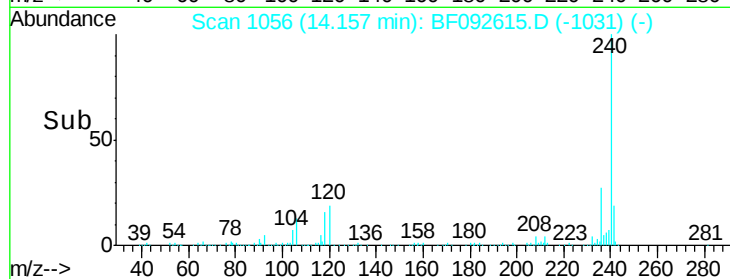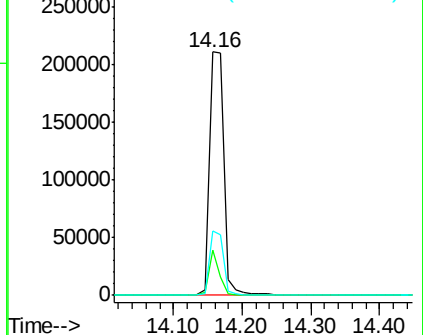

#78

Terphenyl-d14

Concen: 96.43 ng

RT: 13.12 min Scan# 965

Delta R.T. -0.00 min

Lab File: BF092615.D

Acq: 28 Jan 2017 9:44


Tgt Ion:244 Resp: 1126534

Ion Ratio Lower Upper

244 100

212 6.5 6.2 9.2



122 6.7 11.4 17.2#

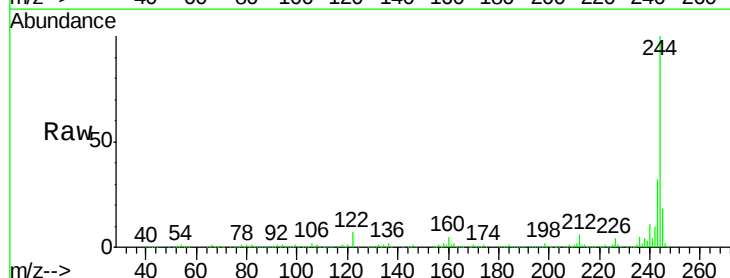


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

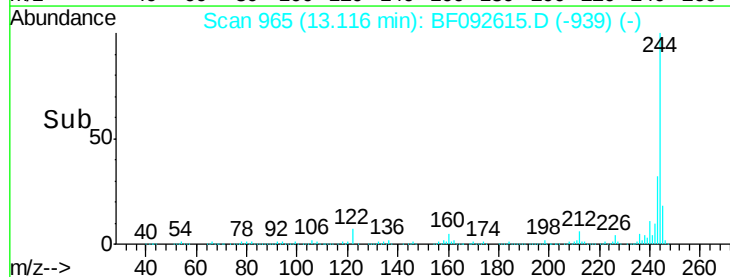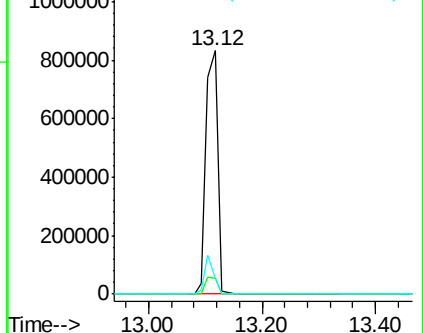


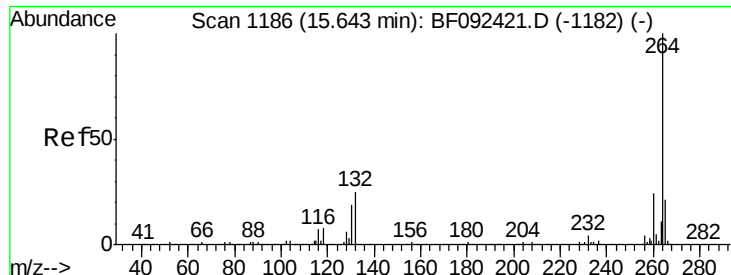

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.65 min Scan# 1187
Delta R.T. 0.01 min
Lab File: BF092615.D
Acq: 28 Jan 2017 9:44

Instrument :
BNA_F
ClientSampleId :
SB-16-COMP

Tgt Ion: 264 Resp: 212929
Ion Ratio Lower Upper
264 100
260 23.6 19.2 28.8
265 21.6 17.4 26.0



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

