
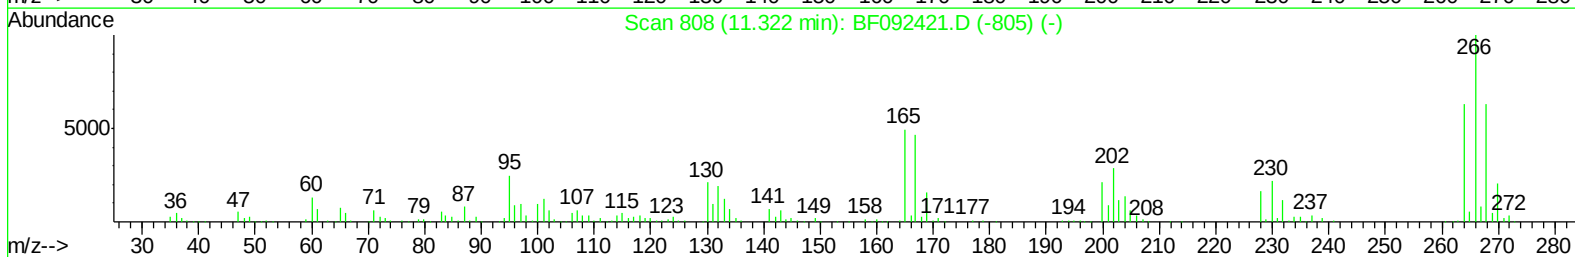
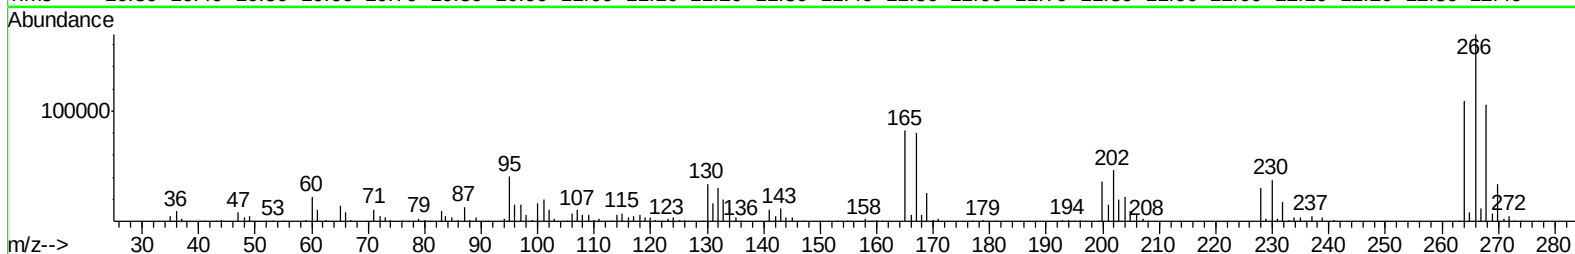


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012717\
Data File : BF092581.D
Acq On : 27 Jan 2017 17:36
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 06:01:07 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

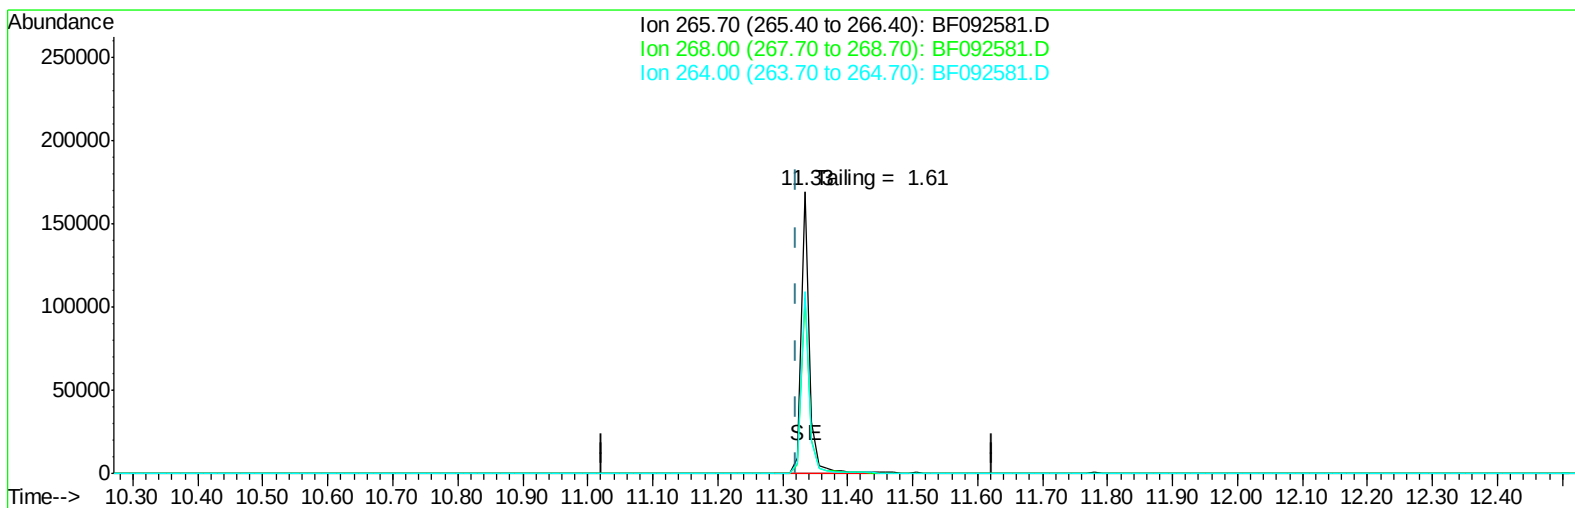

TIC: BF092581.D

(69) Pentachlorophenol (C)




11.334min (+0.011) 0.00ng

response 155342

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.48
264.00	62.90	64.47
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012717\
Data File : BF092581.D
Acq On : 27 Jan 2017 17:36
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 28 06:01:07 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

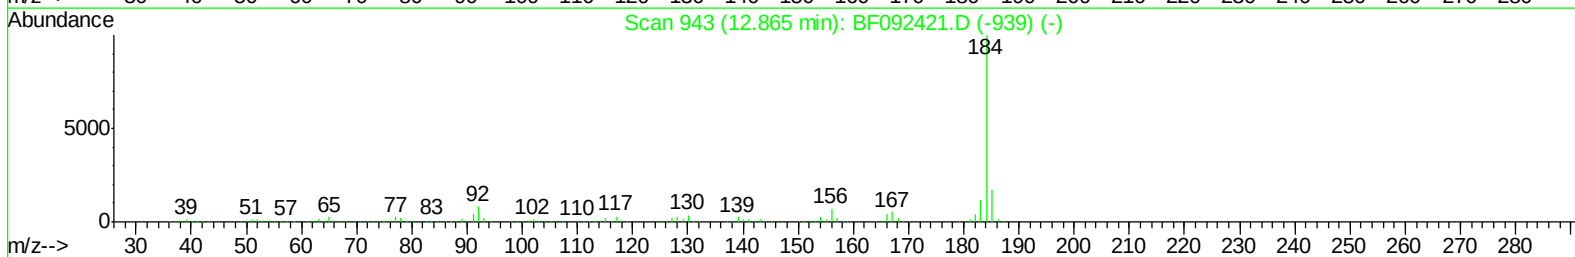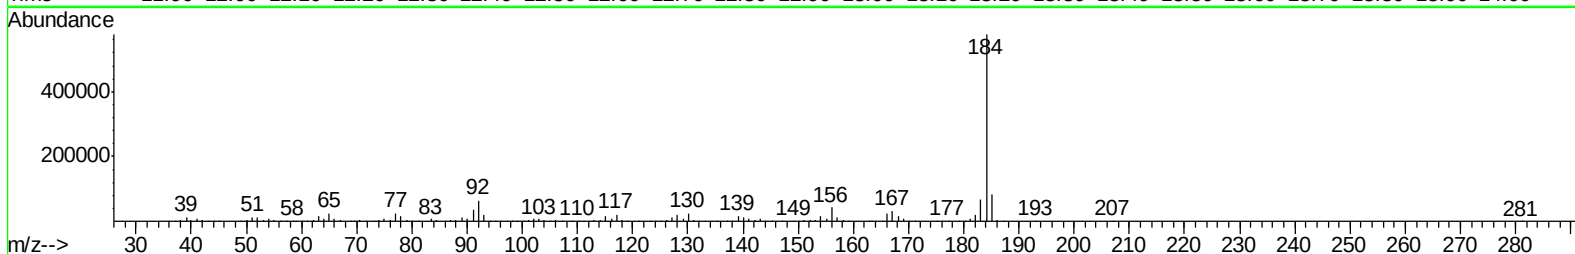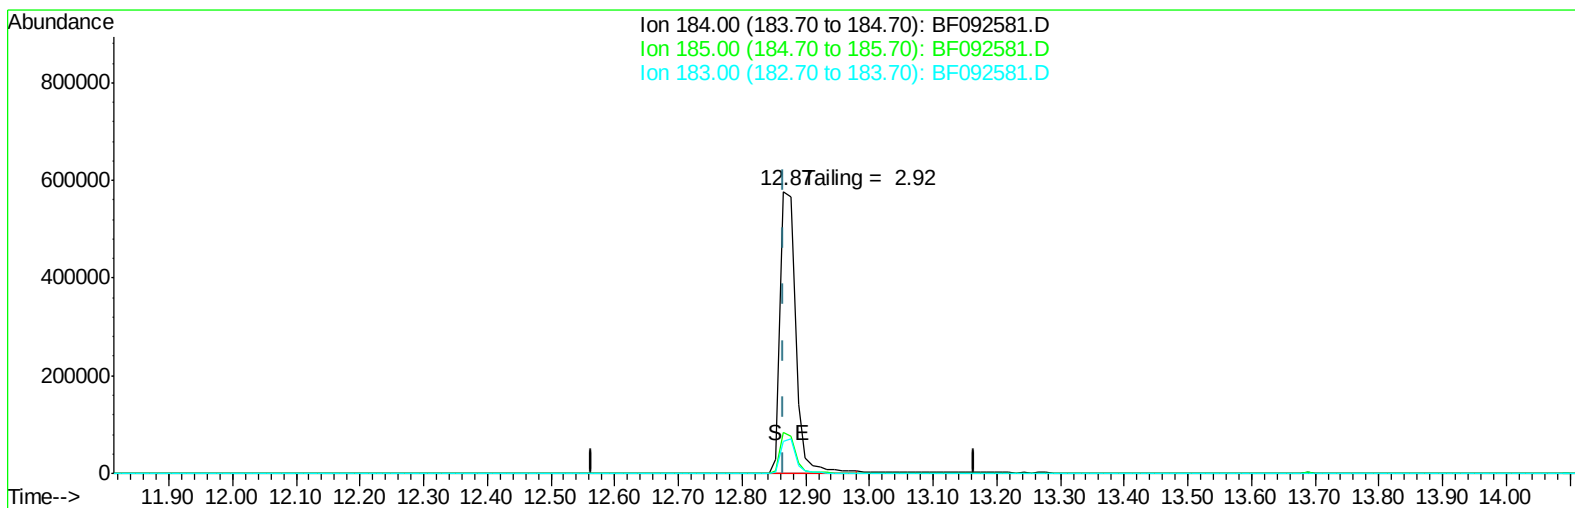

TIC: BF092581.D

(76) Benzidine

12.865min (+0.000) 35769.43ng

response 985284

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.38
183.00	11.50	11.46
0.00	0.00	0.00