
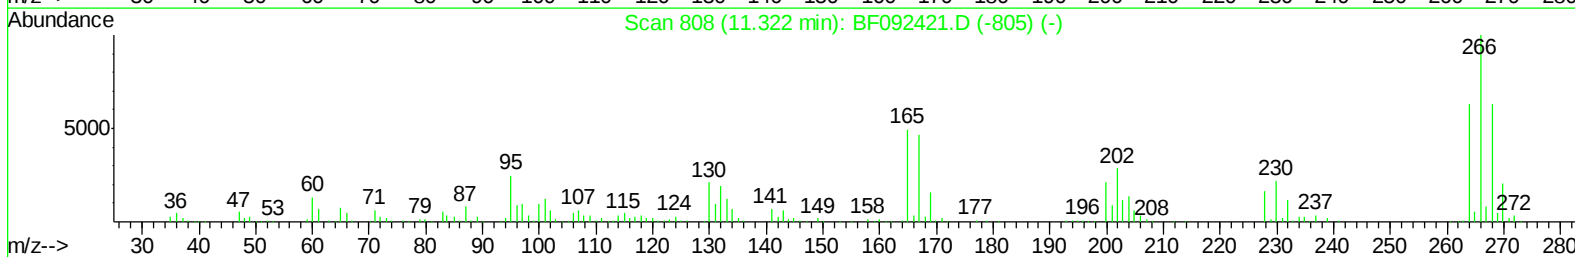
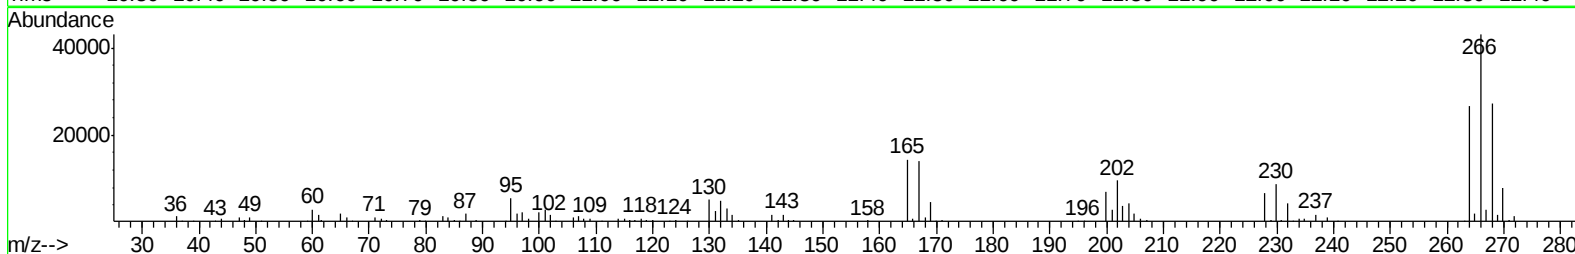


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012717\
Data File : BF092606.D
Acq On : 28 Jan 2017 5:39
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 01:15:22 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

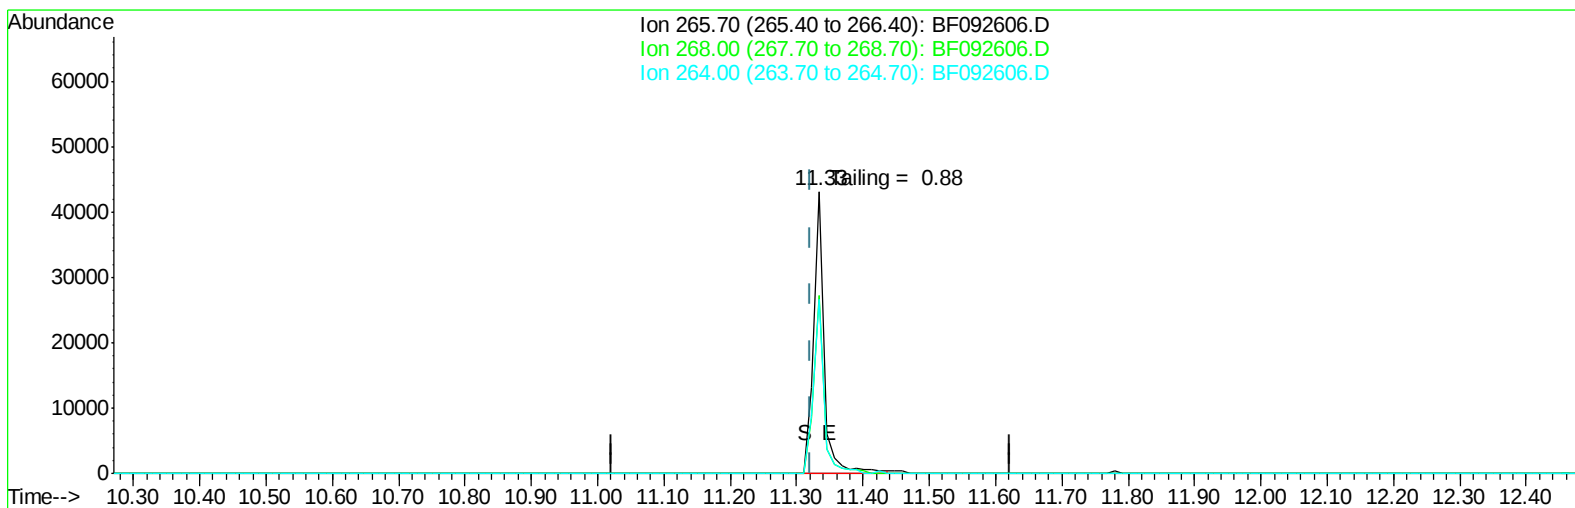

TIC: BF092606.D

(69) Pentachlorophenol (C)




11.333min (+0.011) 0.00ng

response 47651

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	63.37
264.00	62.90	61.79
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012717\
Data File : BF092606.D
Acq On : 28 Jan 2017 5:39
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 30 01:15:22 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

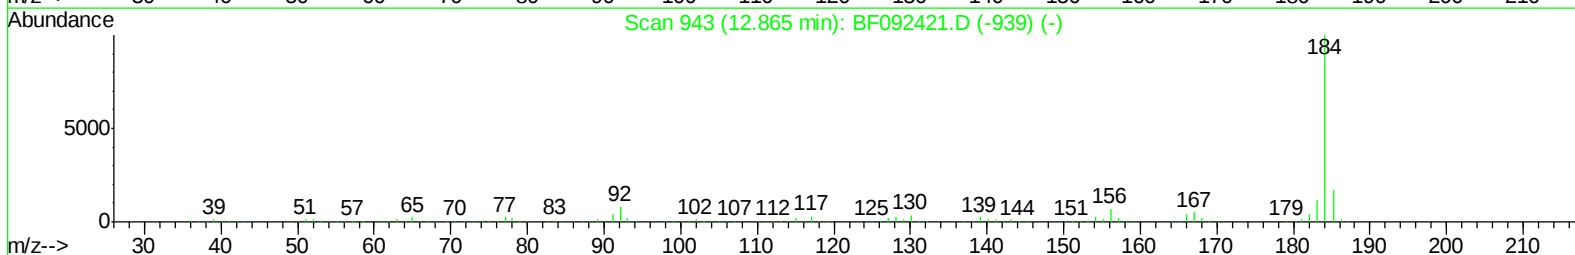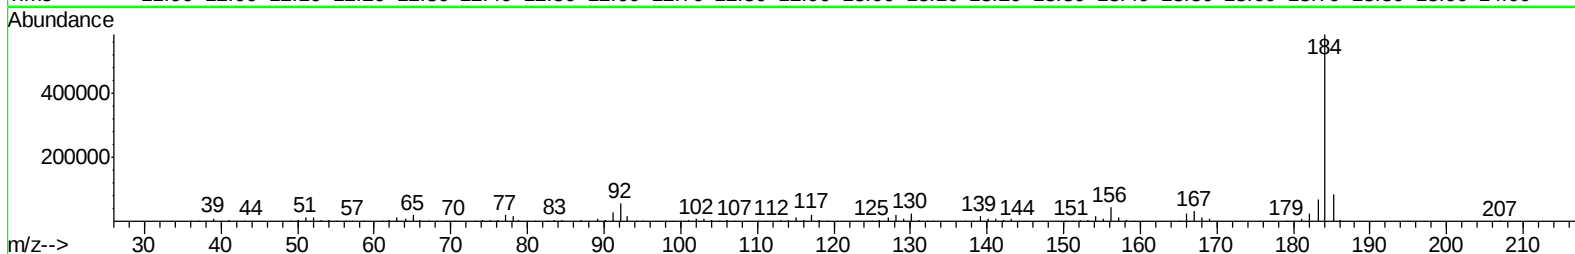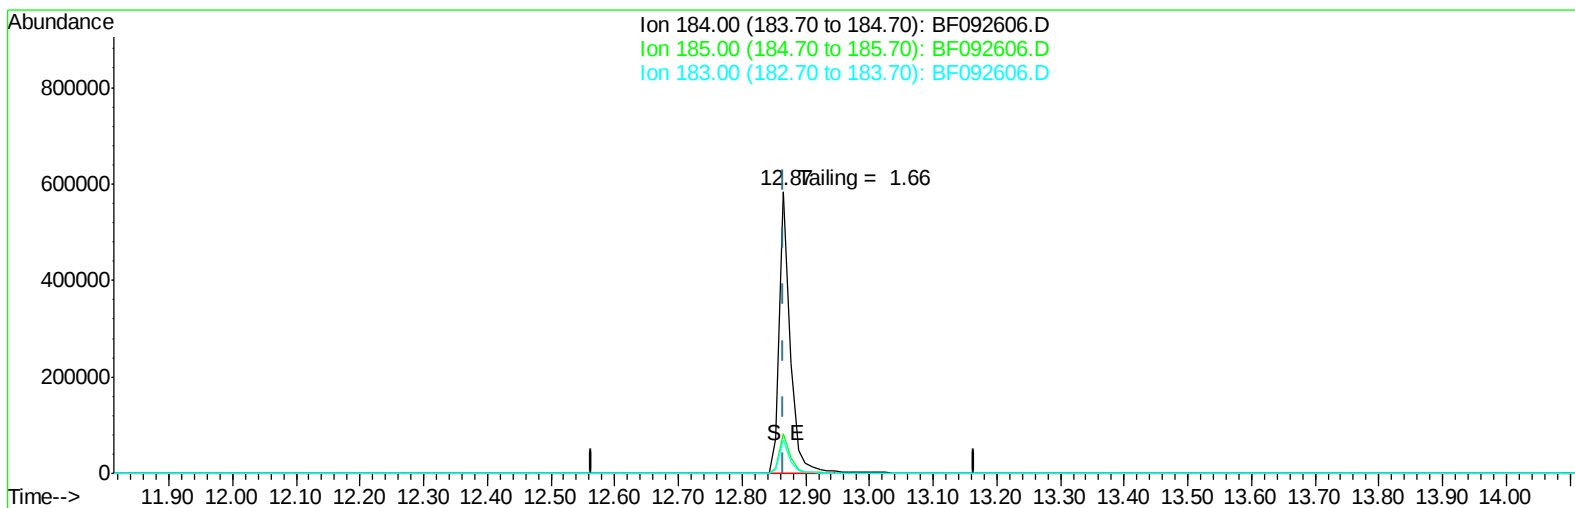

TIC: BF092606.D

(76) Benzidine

12.865min (-0.000) 0.00ng

response 692082

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.26
183.00	11.50	11.78
0.00	0.00	0.00