

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012717\
 Data File : BF092618.D
 Acq On : 28 Jan 2017 11:06
 Operator : SJ/MA
 Sample : I1528-12
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-19-COMP

Quant Time: Jan 30 00:31:09 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 24 13:48:07 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	151092	20.00	ng	0.00
21) Naphthalene-d8	8.27	136	564015	20.00	ng	0.00
38) Acenaphthene-d10	10.03	164	280556	20.00	ng	0.00
63) Phenanthrene-d10	11.52	188	370381	20.00	ng	-0.01
75) Chrysene-d12	14.17	240	320088	20.00	ng	0.00
86) Perylene-d12	15.65	264	225910	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	1341506	138.14	ng	0.05
7) Phenol-d6	6.62	99	1786333	144.41	ng	0.03
23) Nitrobenzene-d5	7.54	82	874342	84.68	ng	0.00
41) 2,4,6-Tribromophenol	10.83	330	232948	121.84	ng	0.01
44) 2-Fluorobiphenyl	9.36	172	1673180	110.28	ng	0.00
78) Terphenyl-d14	13.12	244	1204386	100.19	ng	0.00
Target Compounds						
10) Phenol	6.64	94	55049	3.69	ng	Qvalue # 61
49) Dimethylphthalate	9.74	163	170707	9.57	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF012717\
Data File : BF092618.D
Acq On : 28 Jan 2017 11:06
Operator : SJ/MA
Sample : I1528-12
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-19-COMP

Quant Time: Jan 30 00:31:09 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF012417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 13:48:07 2017
Response via : Initial Calibration

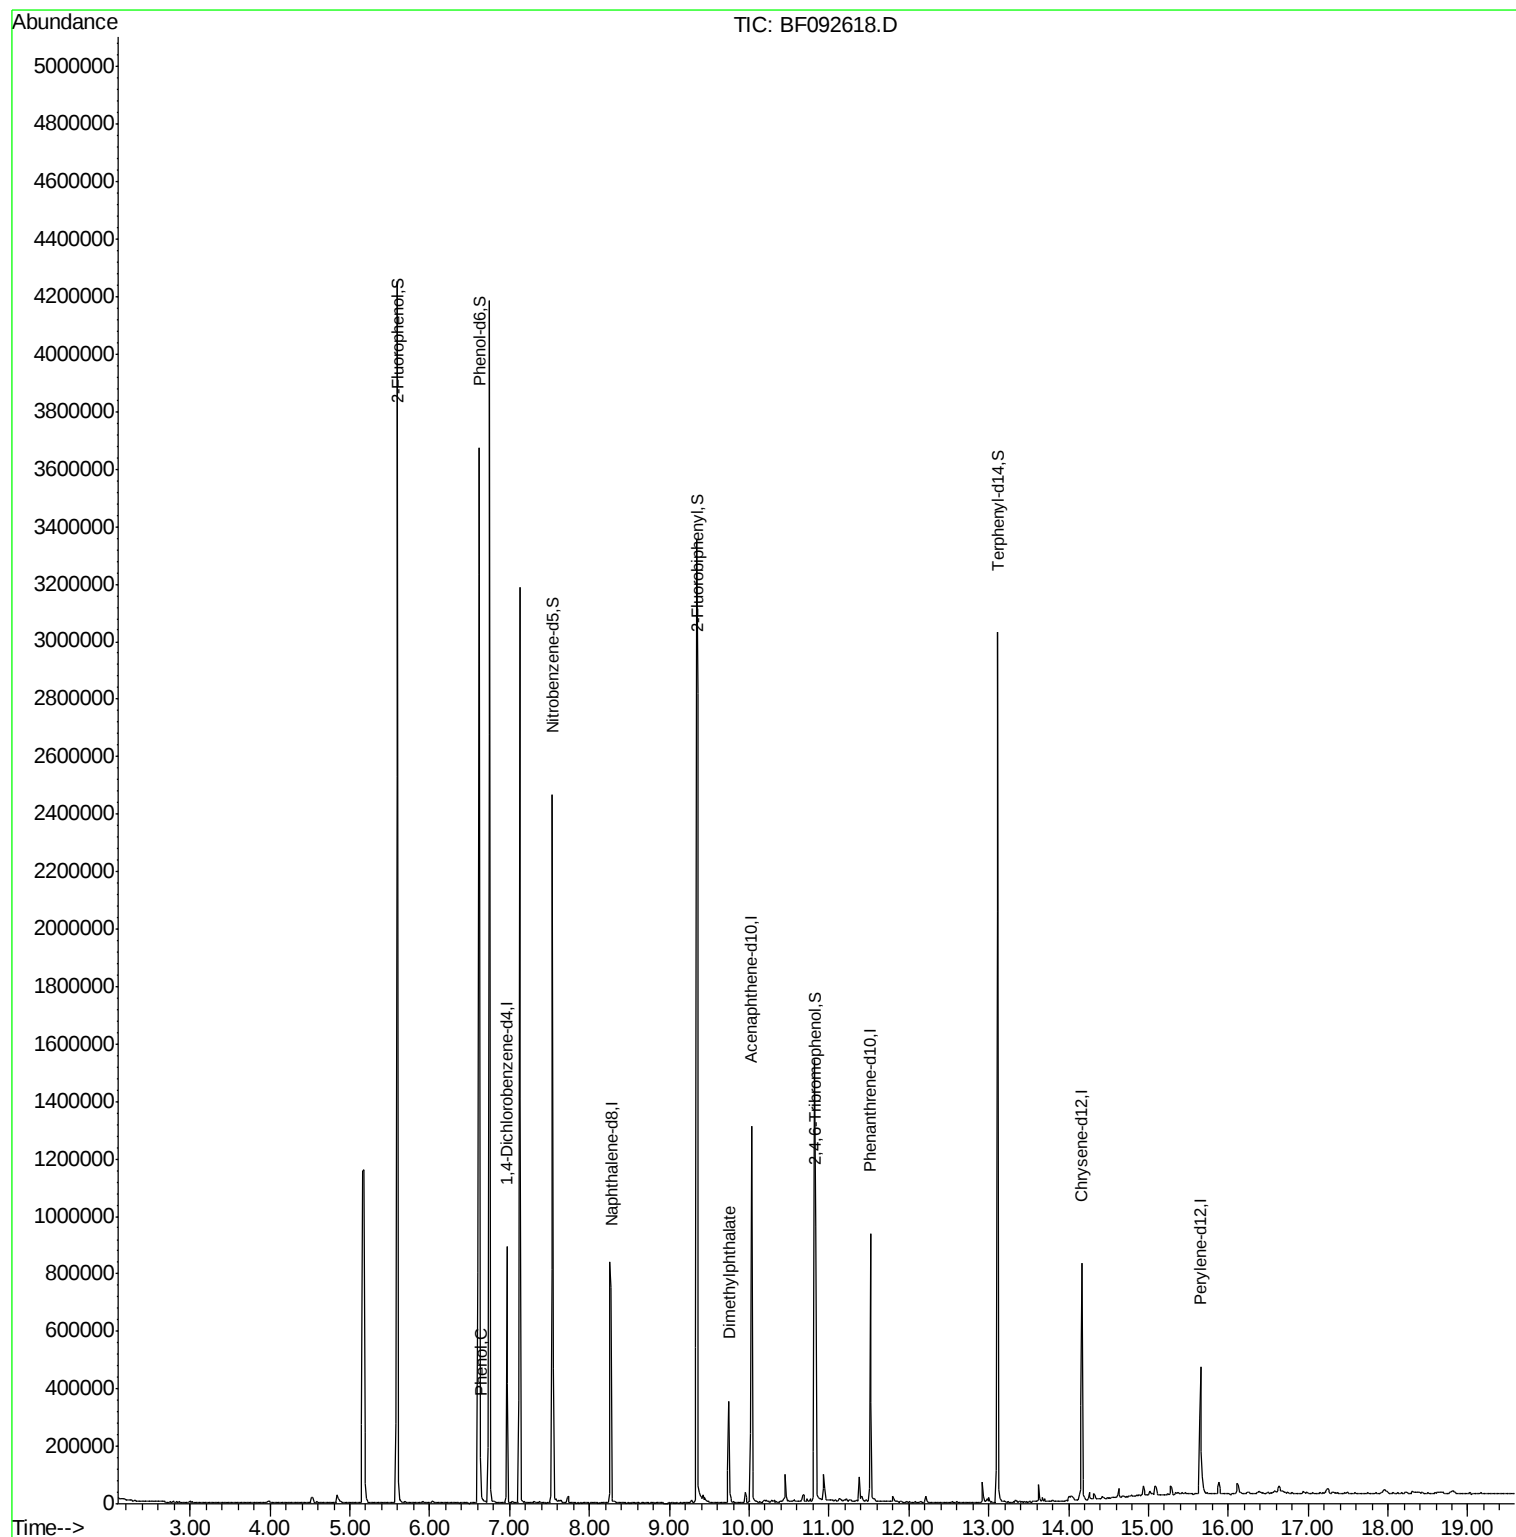



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.97 min Scan# 427

Delta R.T. -0.00 min

Lab File: BF092618.D

Acq: 28 Jan 2017 11:06

Instrument :

BNA_F

ClientSampleId :

SB-19-COMP


Tgt Ion:152 Resp: 151092

Ion Ratio Lower Upper

152 100

150 156.8 124.9 187.3




115 65.3 46.0 69.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

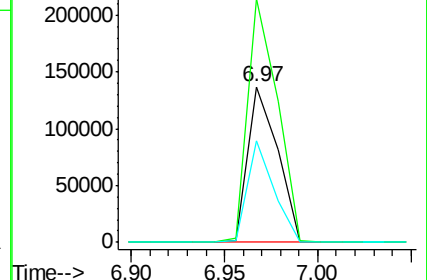

#5

2-Fluorophenol

Concen: 138.14 ng

RT: 5.60 min Scan# 307

Delta R.T. 0.05 min

Lab File: BF092618.D

Acq: 28 Jan 2017 11:06


Tgt Ion:112 Resp: 1341506

Ion Ratio Lower Upper

112 100

64 63.5 46.1 69.1



63 31.8 23.8 35.6




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

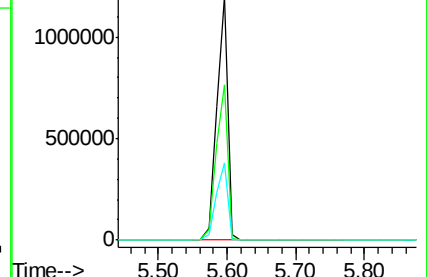

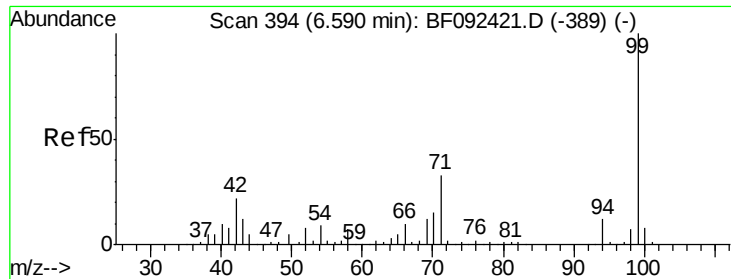

#7

Phenol-d6

Concen: 144.41 ng

RT: 6.62 min Scan# 397

Delta R.T. 0.03 min

Lab File: BF092618.D

Acq: 28 Jan 2017 11:06

Instrument :

BNA_F

ClientSampleId :

SB-19-COMP





Tgt Ion: 99 Resp: 1786333

Ion Ratio Lower Upper

99 100

42 17.6 15.6 23.4

71 30.8 27.5 41.3

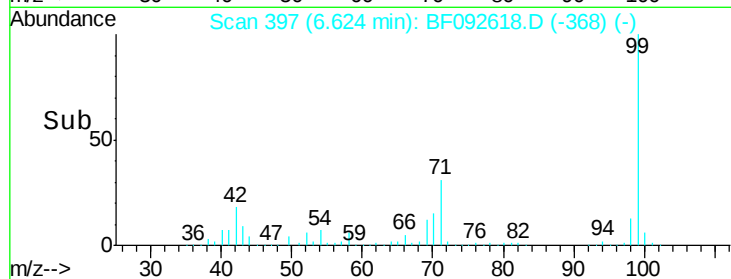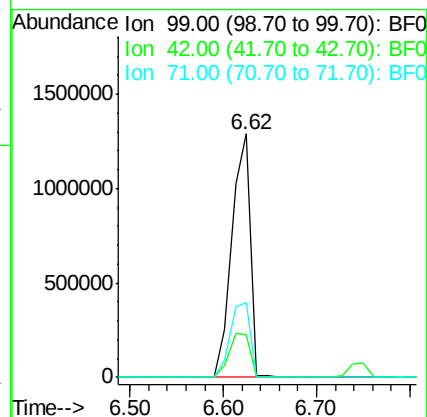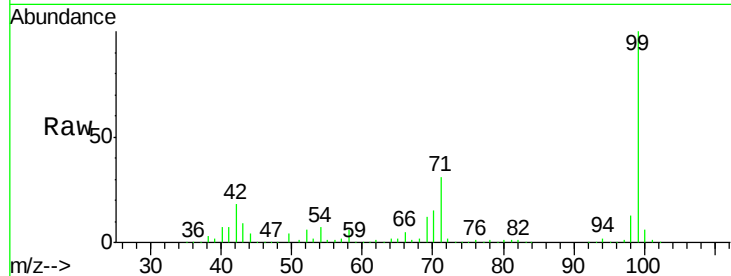

#10

Phenol

Concen: 3.69 ng

RT: 6.64 min Scan# 398

Delta R.T. 0.03 min

Lab File: BF092618.D

Acq: 28 Jan 2017 11:06




Tgt Ion: 94 Resp: 55049


Ion Ratio Lower Upper

94 100

65 22.0 21.4 61.4

66 28.8 44.0 84.0#

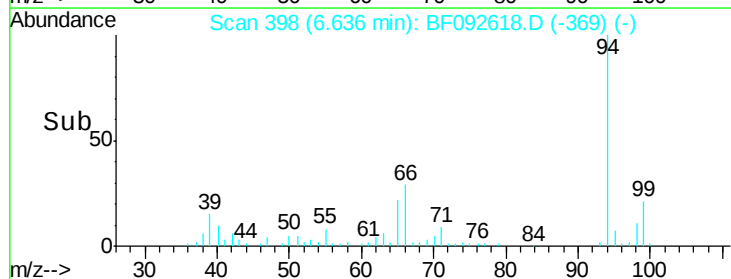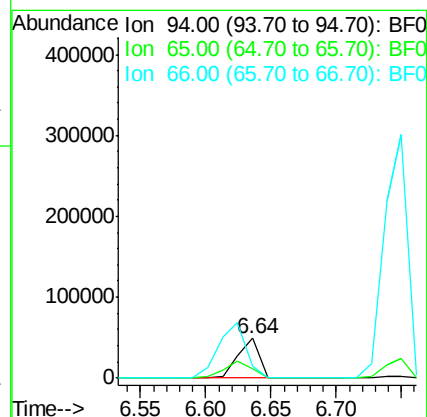


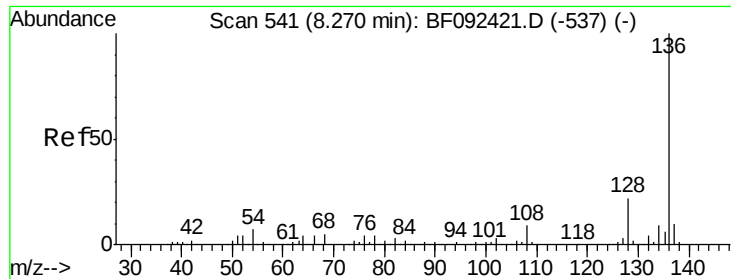




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.27 min Scan# 541
Delta R.T. -0.00 min
Lab File: BF092618.D
Acq: 28 Jan 2017 11:06

Instrument :
BNA_F
ClientSampleId :
SB-19-COMP

Tgt Ion:	136	Resp:	564015
Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.4	12.6
54	6.6	4.5	6.7
68	4.9	3.6	5.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

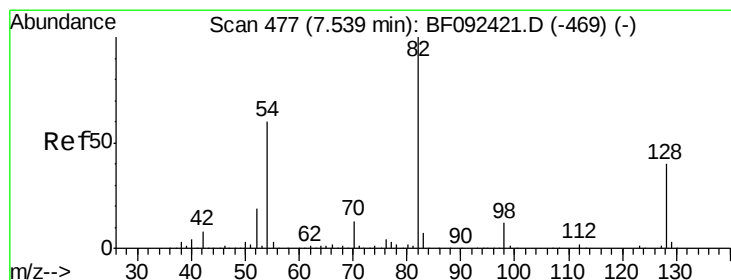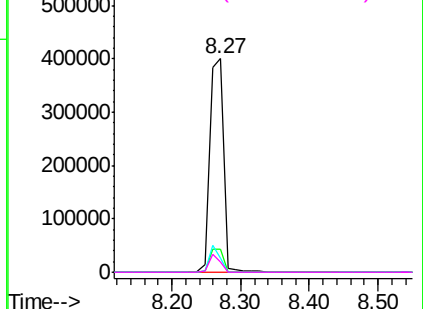




#23
Nitrobenzene-d5
Concen: 84.68 ng
RT: 7.54 min Scan# 477
Delta R.T. -0.00 min
Lab File: BF092618.D
Acq: 28 Jan 2017 11:06

Tgt Ion:	82	Resp:	874342
Ion	Ratio	Lower	Upper
82	100		
128	41.2	34.6	52.0
54	58.5	39.5	59.3



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0



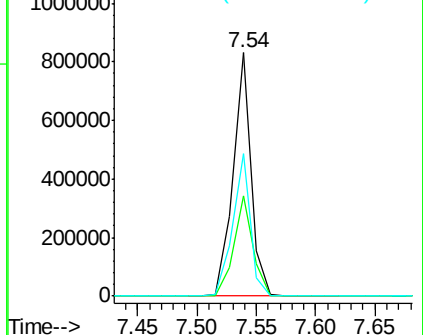
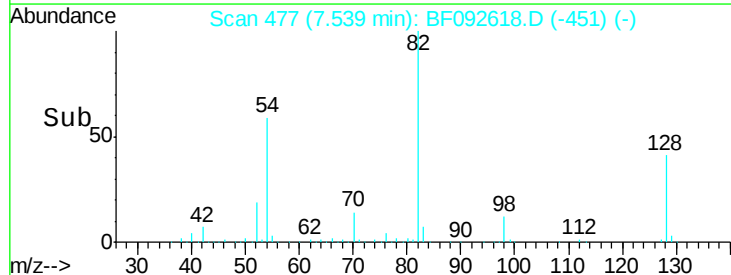


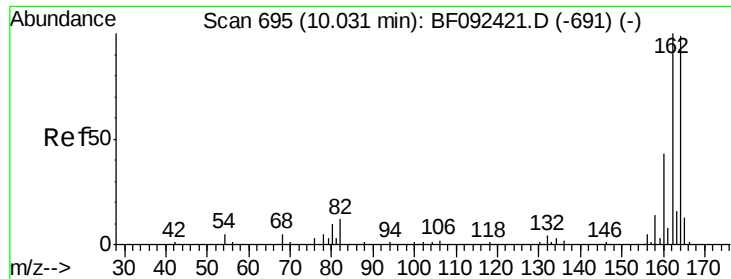

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 10.03 min Scan# 695
Delta R.T. -0.00 min
Lab File: BF092618.D
Acq: 28 Jan 2017 11:06




Instrument :
BNA_F
ClientSampleId :
SB-19-COMP


Tgt Ion:164 Resp: 280556
Ion Ratio Lower Upper
164 100
162 100.7 80.2 120.2
160 42.8 36.9 55.3

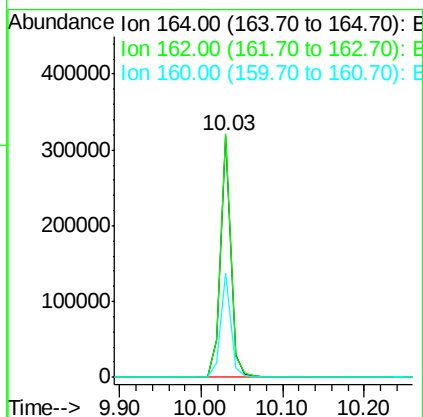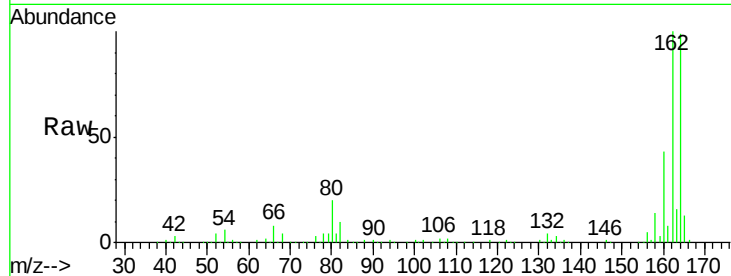

#41
2,4,6-Tribromophenol
Concen: 121.84 ng
RT: 10.83 min Scan# 765
Delta R.T. 0.01 min
Lab File: BF092618.D
Acq: 28 Jan 2017 11:06

Tgt Ion:330 Resp: 232948
Ion Ratio Lower Upper
330 100
332 98.3 77.4 116.2
141 34.3 34.1 51.1

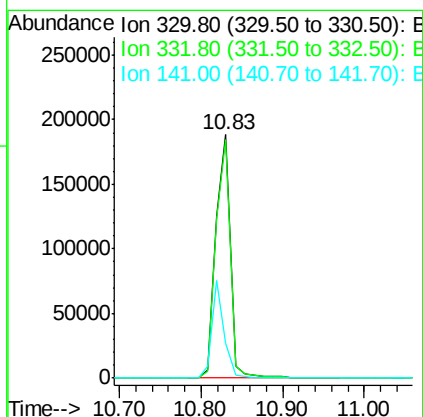







#44
 2-Fluorobiphenyl
 Concen: 110.28 ng
 RT: 9.36 min Scan# 636
 Delta R.T. -0.00 min
 Lab File: BF092618.D
 Acq: 28 Jan 2017 11:06

Instrument :
 BNA_F
 ClientSampleId :
 SB-19-COMP

Tgt Ion:172 Resp: 1673180
 Ion Ratio Lower Upper
 172 100
 171 35.6 29.4 44.0
 170 23.8 20.2 30.4




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

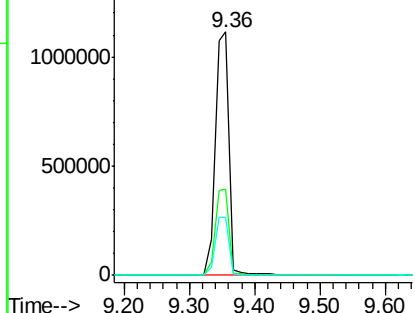




#49
 Dimethylphthalate
 Concen: 9.57 ng
 RT: 9.74 min Scan# 670
 Delta R.T. -0.01 min
 Lab File: BF092618.D
 Acq: 28 Jan 2017 11:06

Tgt Ion:163 Resp: 170707
 Ion Ratio Lower Upper
 163 100
 194 3.6 3.0 4.4
 164 10.0 8.0 12.0



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

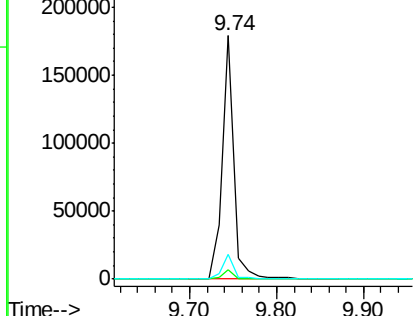







#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.52 min Scan# 825
 Delta R.T. -0.01 min
 Lab File: BF092618.D
 Acq: 28 Jan 2017 11:06

Instrument :
 BNA_F
 ClientSampleId :
 SB-19-COMP

Tgt Ion:188 Resp: 370381
 Ion Ratio Lower Upper
 188 100
 94 13.1 10.0 15.0
 80 14.4 11.2 16.8

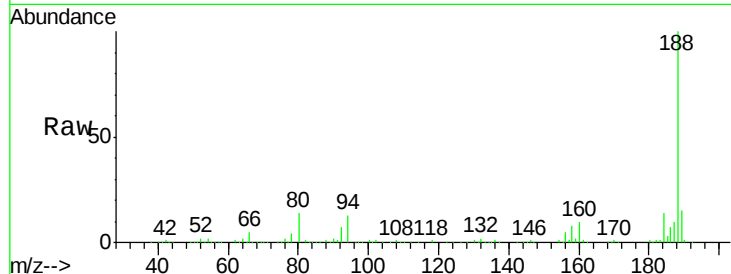


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0


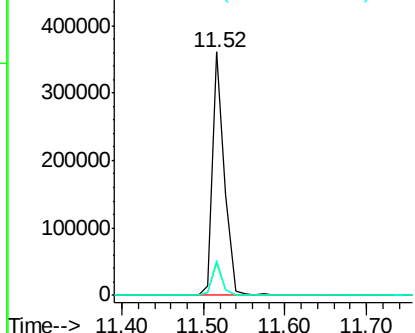



#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 14.17 min Scan# 1057
 Delta R.T. -0.00 min
 Lab File: BF092618.D
 Acq: 28 Jan 2017 11:06

Tgt Ion:240 Resp: 320088
 Ion Ratio Lower Upper
 240 100
 120 10.0 12.9 19.3#
 236 25.9 20.9 31.3

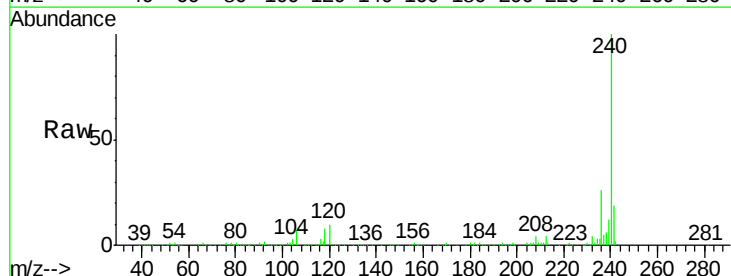

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

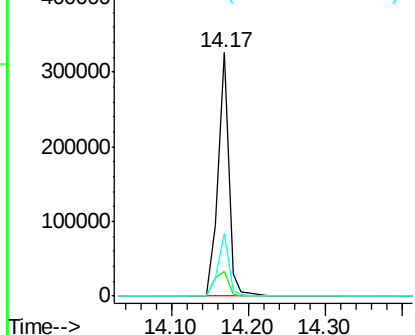







#78
 Terphenyl-d14
 Concen: 100.19 ng
 RT: 13.12 min Scan# 965
 Delta R.T. -0.00 min
 Lab File: BF092618.D
 Acq: 28 Jan 2017 11:06

Instrument :
 BNA_F
 ClientSampleId :
 SB-19-COMP

Tgt Ion:244 Resp: 1204386
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.2 9.2
 122 8.7 11.4 17.2#




Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

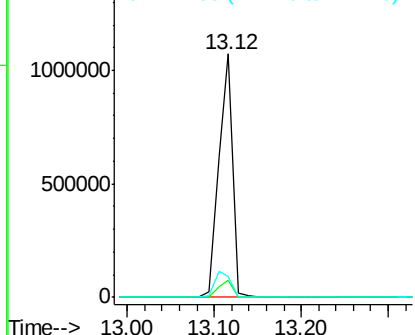

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.65 min Scan# 1187
 Delta R.T. 0.01 min
 Lab File: BF092618.D
 Acq: 28 Jan 2017 11:06

Tgt Ion:264 Resp: 225910
 Ion Ratio Lower Upper
 264 100
 260 23.8 19.2 28.8
 265 21.5 17.4 26.0



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

